

Type ML-x17, ML-x15, WDL-x14, ML-2013**Low power 2G/3G/4G data loggers**

Title : User Manual ML-x17, ML-x15, WDL-x14, ML-2013 **Date** : March-2019

Version : FW V3.5B5

WARNING

THE FOLLOWING OPERATING INSTRUCTIONS ARE FOR USE BY QUALIFIED PERSONNEL ONLY. TO AVOID DAMAGE OR MALFUNCTION, DO NOT PERFORM ANY OPERATING OTHER THAN THAT CONTAINED IN THIS MANUAL. ANY OPERATOR SHOULD BE SKILLED WITH A TECHNICAL BACKGROUND BEFORE OPERATING THE DEVICE.

PREFACE

Congratulations!

With your purchase of an YDOC Low Power data logger with mobile network capabilities.

This manual describes the operation and (hardware) installation of the ML-2013/ML-x15/ML-x17/WDL-x14 data logger.

The chapter *Getting Started* briefly describes the data logger, prepares you to install it, and tells you how to put it into operation.

The Chapter *Operating Basics* covers basic principles of operation of the data logger. The operating interface (menu) and the tutorial examples, rapidly help you to understand how your data logger operates.

The Chapter *Reference* teaches you how to perform specific tasks and provides a complete list of operating tasks and useful background information.

The Appendices provide a list with all available options, and other useful information.

We recommend reading this manual carefully before installation of the data logger.

Warranty

All YDOC instruments are warranted for 3 years against defective materials and workmanship. Any questions with respect to the warranty mentioned above should be taken up with your YDOC Distributor.

Table of Contents

1.	Product description.....	10
1.1	Models and Editions	11
1.1.1	ML-2013.....	11
1.1.2	ML-x15.....	12
1.2	ML-x17.....	14
1.3	WDL-x14.....	16
2	Getting started.....	18
2.1	Vibration.....	18
2.2	Do's & Don'ts	18
2.3	Inserting the SIM-card	18
2.4	Power on for the First time.....	19
2.5	Connect to a PC	19
3	Operating Basics	20
3.1	Configuration menu	20
4	Reference.....	27
4.1	Principle of Operation	27
4.1.1	Intervals	27
4.1.1.1	Sample interval.....	27
4.1.1.2	Data logging interval.....	27
4.1.1.3	Send Interval.....	27
4.1.1.4	Example.....	27
4.1.2	Common data output settings.....	28
4.1.2.1	Send delay.....	28
4.1.2.2	Output type	28
4.1.2.3	Data format	28
4.1.2.4	Data filter.....	28
4.2	Parameters	29
4.2.1	Name	29
4.2.2	Code	29
4.2.3	Unit.....	29
4.2.4	Value factor.....	29
4.2.5	Value offset.....	29
4.2.6	Decimals	29
4.2.7	Data log.....	29
4.2.8	Data transpond	30
4.2.9	Alarm message.....	30
4.2.10	Alarm log.....	30
4.2.11	Alarm output.....	30
4.2.12	Alarm limits and delays.....	30
4.3	Configuration Menu Settings	31
4.3.1	Date & Time.....	31
4.3.2	System Information.....	31
4.4	Configuration Setup	32
4.5	General Settings	33
4.5.1	Exit.....	33
4.5.2	System Name	33
4.5.3	Data log interval.....	33
4.5.3.1	Normal mode	33
4.5.3.2	Alarm mode.....	33
4.5.4	Timestamp round down	33
4.5.5	Continuous Alarm Sampling	33
4.5.6	Alarm output port	34
4.5.7	Battery protection.....	34
4.5.8	Deployment Date and Time.....	34
4.5.9	Daily operating time slot	34

4.5.10	Time zone	34
4.5.11	Summer time.....	34
4.6	Modem Settings.....	35
4.6.1	Provider Selection.....	35
4.6.2	Access Point Name (APN).....	35
4.6.3	APN Authentication.....	35
4.6.4	Network signal test	35
4.6.5	APN login test	36
4.7	NTP time update.....	36
4.7.1	Time Update	36
4.7.2	Update interval.....	36
4.7.3	Server	36
4.7.4	NTP Port	36
4.7.5	Time update test	36
4.8	Alarm messages	36
4.8.1	System Alarm	36
4.8.2	Data Alarm.....	36
4.9	Option boards (ML-x17 only)	37
4.9.1	Calibration.....	37
4.9.2	Zero-calibration	37
4.10	Internal Sensors.....	38
4.10.1	Name	38
4.10.2	Sample interval	38
4.10.3	Battery Capacity	38
4.10.4	Battery Replaced	38
4.10.5	Rest Capacity	38
4.10.6	Rest power.....	38
4.10.7	Inner Pressure	39
4.10.8	Inner Temperature	39
4.10.9	Processor Temperature	39
4.10.10	Average Voltage	39
4.10.11	Max Voltage.....	39
4.10.12	Min Voltage.....	39
4.10.13	Average, Max, Min current.....	39
4.10.14	Operating cycle.....	39
4.10.15	Free disk space	39
4.11	Analog inputs	40
4.11.1	Sensor power switch.....	40
4.11.2	Sample interval	40
4.11.3	Port mode	40
4.11.4	Parameter settings.....	40
4.11.5	Parameter value at (min & max range).....	40
4.11.6	Determine linear conversion function (2 calibration points).....	40
4.11.7	Determine linear offset only (1 calibration point)	40
4.12	Digital inputs – Pulse counter	41
4.12.1	Sample interval	41
4.12.2	Port mode	41
4.12.2.1	Pull up.....	41
4.12.2.2	Pull down	42
4.12.3	Register mode	42
4.12.4	Units per pulse, or pulses per unit	42
4.12.5	Register value.....	42
4.12.6	Register Reset	42
4.12.7	Log each counter change	42
4.12.8	Counter	42
4.12.9	Quantity.....	42
4.12.10	Mean-, Max- and Min Rate	42

4.13	Digital inputs - Alarm trigger	43
4.13.1	Trigger delay	43
4.13.2	Register value	43
4.14	Digital inputs - State input / On-time meter.....	44
4.14.1	Total On-time	44
4.14.2	Register value	44
4.14.3	Register reset	44
4.14.4	Interval On-time	44
4.14.5	Input state	44
4.15	Network Signal Sensor	45
4.15.1	Independent data log	45
4.15.2	Signal bars	45
4.15.3	Signal dB%/indication/bit error rate	45
4.16	Aggregation Channels	46
4.16.1.1	Average, minimum, maximum and standard deviation	47
4.16.1.2	Percentiles	47
4.17	Calculation Channels	47
4.17.1	Syntax	48
4.17.2	Functions	48
4.17.3	Example 1	48
4.17.4	Example 2	48
4.17.5	Supported mathematical functions with one argument:	49
4.17.5.1	abs(x)	49
4.17.5.2	sqrt(x)	49
4.17.5.3	ln(x)	49
4.17.5.4	exp(x)	49
4.17.5.5	log(x)	49
4.17.5.6	sin(radians)	49
4.17.5.7	cos(radians)	49
4.17.5.8	tan(radians)	49
4.17.5.9	asin(x)	49
4.17.5.10	acos(x)	49
4.17.5.11	atan(x)	49
4.17.5.12	torad(degrees)	50
4.17.5.13	todeg(radians)	50
4.17.5.14	floor(x)	50
4.17.5.15	ceil(x)	50
4.17.5.16	round(x)	50
4.17.6	Supported mathematical functions with multiple arguments:	50
4.17.6.1	atan2(x;y)	50
4.17.6.2	mod(x;y)	50
4.17.6.3	pow(x;y)	50
4.17.6.4	clip(x;min;max)	50
4.17.7	Supported comparisons with 2 arguments:	50
4.17.7.1	lt(x;y)	50
4.17.7.2	le(x;y)	50
4.17.7.3	gt(x;y)	50
4.17.7.4	ge(x;y)	50
4.17.8	Supported comparisons with 4 arguments:	51
4.17.8.1	eq(x;y;q;p)	51
4.17.8.2	lt(x;y;q;p)	51
4.17.8.3	le(x;y;q;p)	51
4.17.8.4	gt(x;y;q;p)	51
4.17.8.5	ge(x;y;q;p)	51
4.17.9	Various supportive functions:	51
4.17.9.1	pi	51
4.17.9.2	time	51

4.18	Serial Port	52
4.18.1	RS232	52
4.18.2	Generic Modbus	52
4.18.2.1	Port Settings	52
4.18.2.2	Protocol type	52
4.18.2.3	Start command	53
4.18.2.4	Ready status	53
4.18.2.5	Ready after	53
4.18.2.6	Register type	53
4.18.2.7	Register Start address	53
4.18.2.8	Data Type	53
4.18.2.9	Timing	53
4.18.3	Generic Serial	54
4.18.3.1	Log raw data String	54
4.18.3.2	Decimal symbol	54
4.18.3.3	Separator Character	54
4.18.3.4	Start/Stop character	54
4.18.3.5	Output request	54
4.18.3.6	Parameters	55
4.18.3.7	Sentence filter	55
4.18.3.8	Field position	55
4.18.3.9	Field type	55
4.18.3.10	Example:	55
4.18.4	Generic NMEA	55
4.18.4.1	GPS	56
4.18.5	RS485	56
4.18.6	SDI-12	56
4.18.6.1	Measurement command	56
4.18.6.2	Parameters	56
4.18.7	Accessory port	57
4.18.8	Radio	57
4.18.8.1	Send interval	57
4.18.8.2	Send delay	57
4.18.8.3	Power down delay	57
4.18.9	Iridium Satellite	58
4.18.9.1	Iridium SBD Service	58
4.18.9.2	Settings menu	59
4.18.9.3	Send interval	59
4.18.9.4	Data transpond	59
4.18.9.5	Backup mode	59
4.18.9.6	Message format	59
4.18.10	GPS	60
4.18.10.1	Minimum satellites to use	60
4.18.10.2	Time to fix	60
4.18.10.3	Position drift alarming	60
4.18.10.3.1	Calculate alarm limits on deployment	61
4.18.10.3.2	Latitude/Longitude hi/lo alarm drift	61
4.18.10.4	Satellites	61
4.18.10.5	Latitude / Longitude	61
4.18.10.6	GPS Quality	61
4.18.11	Camera	62
4.18.12	Display	63
4.18.12.1	Power down delay	63
4.18.12.2	Order of parameters	63
4.19	Email output	64
4.19.1	Server	64
4.19.2	SMTP port	64

4.19.3	Security	64
4.19.4	Originator address	64
4.19.5	Destination address	64
4.19.6	Remote configuration.....	64
4.20	FTP Output	65
4.20.1	Server	65
4.20.2	Port	65
4.20.3	FTP mode	65
4.20.4	Security	65
4.20.5	Directory.....	65
4.20.6	File name	65
4.20.7	Remote configuration.....	66
4.21	HTTP Output.....	67
4.21.1	Server	67
4.21.2	TCP port.....	67
4.21.3	Security	67
4.21.4	Data format	67
4.21.5	Remote configuration.....	68
4.22	MQTT Output.....	69
4.22.1	Server	69
4.22.2	Port	69
4.22.3	Security	69
4.22.4	Root topic.....	69
4.22.5	Client ID	70
4.22.6	Clean Session.....	70
4.22.7	Max Payload	70
4.22.8	Remote configuration transfer and firmware upgrade	71
4.22.9	Remote configuration.....	72
4.23	TCP Output	73
4.23.1	Server	73
4.23.2	Port	73
4.23.3	Security	73
4.24	SMS output	74
4.24.1	Phone number	74
4.24.2	Data send.....	74
4.24.3	Data format	74
4.24.4	Remote configuration.....	74
4.25	Satellite Output (SBD)	74
4.26	Parameter overview	75
4.26.1	Parameter list.....	75
4.26.2	Measurement list	75
4.26.3	Alarm list	76
4.26.4	Alarm limits	76
4.27	Maintenance Menu	77
4.27.1	Field Testing	77
4.27.1.1	Verify Analog inputs.....	77
4.27.1.2	Digital input test	77
4.27.1.3	SD card test	78
4.27.1.4	Battery test.....	78
4.27.1.5	Comport redirect	78
4.27.1.6	Data Download	79
4.27.1.7	Format SD Card.....	79
4.27.1.8	Configuration Down/upload	79
4.27.1.9	Firmware Upgrade	80
4.27.1.10	Modem Maintenance	80
4.27.1.11	Bootloader Menu	80
4.28	SDI-12.....	81

4.28.1	SDI-12 Hardware	81
4.28.2	SDI-12 Wiring	81
4.28.3	SDI-12 Baud Rate and Frame Format.....	81
4.29	RS232.....	82
4.30	RS485.....	82
4.31	Analog Inputs (4..20mA).....	84
4.31.1	Loop Powered Devices.....	84
4.31.2	Analog Inputs (0 .. 10 V)	84
4.32	Analog Differential Inputs (ML-2013 only)	84
4.32.1	Differential input ports theory of operation.....	84
4.32.2	Common mode noise rejection	84
4.32.3	Using Load Cells With the ML-2013.....	85
4.32.4	Bridge of Wheatstone	85
4.32.5	Excitation Output.	85
4.32.6	Analog Differential input 5.....	86
4.32.7	Analog Differential input 6.....	86
4.32.8	Calibration of Differential inputs.....	86
4.32.9	Overall Calibration	86
4.33	Potentiometer input (ML-x15 only)	87
4.34	Digital inputs	88
4.34.1	Pull up type	88
4.34.2	Pull down type	88
4.34.3	Electrical specifications Digital inputs.....	88
4.35	Coil input.....	88
4.36	Alarming.....	89
4.36.1	Alarming - principal of operation	89
4.36.2	Advanced Alarming.....	91
4.37	Firmware Upgrade	92
4.37.1	When to use Firmware upgrades.....	92
4.37.2	Firmware upgrade procedure	92
4.37.3	Firmware upgrade over the air	92
4.37.4	Firmware Driver limitations	92
4.37.5	Power Switch Limitations.....	93
4.37.6	Modem.....	93
4.37.7	Modem Firmware Upgrade.....	93
4.38	SD-card.....	93
4.38.1	Inserting an SD-card.....	94
4.39	Native TXT Data Format.....	94
4.39.1.1	Header:	94
4.39.1.2	Parameter Code:	94
4.39.1.3	Parameter Name:	94
4.39.1.4	Parameter Unit:.....	94
4.39.2	D-Records.....	95
4.39.2.1	Parameter Code:	95
4.39.2.2	Parameter value:	95
4.39.3	System records.....	95
4.39.4	Data Modifiers.....	96
4.40	JSON Data Format	97
4.41	Compacted Data Format	98
4.41.1	Records.....	99
4.41.1.1	First byte of record	99
4.41.1.2	Number-bytes	99
4.41.1.3	Time-record.....	100
4.41.1.4	Value-record	100
4.42	Input-drivers.....	101
4.42.1	Analog sensors	101
4.42.2	Digital Pulse Sensor	102

4.42.2.1	Example configuration Rain Measurement.....	102
4.42.2.2	Counter	103
4.42.2.3	Quantity.....	103
4.42.2.4	Rate	104
4.43	Power supply	105
4.43.1	Internal RTC backup battery.....	105
4.43.2	Power consumption & Battery Life	105
5	Pin configuration.....	106
	ML-2013.....	106
5.1	ML-x15/x17	107
5.2	WDL-x14.....	108
5.3	Pin descriptions	109
5.3.1	Analog Inputs.....	109
5.3.1.1	0/4..20mA inputs.....	109
5.3.1.2	0...10V inputs	109
5.3.1.3	Potentiometer input.....	109
5.3.2	RS485 A & B.....	109
5.3.3	Power Switch	109
5.3.4	VBAT +	109
5.3.5	RS232 RX & TX.....	109
5.3.6	SDI-12 Hi	109
5.3.7	Digital inputs	110
5.3.8	+3V6	110
5.3.9	Antenna placement and field strength	110
6	Maintenance and Repair	111
6.1	RTC Lithium Battery replacement	111
6.2	Recalibration.....	111
6.3	XRAY	111
7	Safety	112
7.1	Power supply	112
7.2	ESD.....	112
8	Environment and disposal	112
9	Transport and Storage	112
10	Appendix.....	113
10.1	Specifications.....	113
10.2	CE Declarations of Conformity	114
10.3	Open Collector output.....	118
10.3.1.1.1	Using a relay to drive an external load	118
10.4	Trouble shooting	119
10.5	System messages	120

1. Product description

The data logger is designed to retrieve, and store data from various sensors. This data is logged onto the embedded / removable SD-card. Also, the stored data can be send from the data logger to any remote computer you like. To use this feature, you need a valid SIM-card. Contact your local telecommunications provider for more information on the SIM card you will need. The unit accepts various power sources, selectable by the different version types. The user should connect his sensor(s) of preference to the connector board of the device. Captured data can be stored, send, visualized and manipulated in many ways.

The data logger is a small, ultra-low power, high-end data logger with built-in 2G/3G/4G cellular-modem. This small data logger, is further provided with an internal temperature sensor, 2 or 4 GB micro SD-card and an SIM card slot. The logger can be powered by an internal 3.6 Volt Lithium battery that will last for years when the logger is configured in a low-power mode.

Depending on model and edition a data logger can acquire physical signals by current loop inputs, voltage inputs, potentiometer input and digital inputs. They can also be provided with RS232/RS485/SDI-12 port to capture serial data (ASCII, MODBUS-RTU/ASCII, NMEA-0183, SDI-12) or to connect an accessory (Camera, Display, GPS, Satellite modem).

External sensors can be powered by the data logger itself, to prevent them to consume power while the data logger is a sleep. The excitation voltage is switched off during sleep as well.

Key features:

- A maximum sample rate of 4 Hz,
- Recording buffer up to 4 GB,
- Analog inputs (Except DS editions),
- Serial port(s) (Except AD editions),
- Digital input(s)
- Digital output
- Internal micro SD-card with standard FAT-32 File system for easy use with a PC,
- Easy configuration by menu items of embedded terminal application,
- Can be used with Windows XP, W7, W8 and W10
- Low power / long Battery life (see specification sheet),
- Embedded 2G/3G/4G modem for remote operation,
- Alarming by SMS, e-Mail or MQTT
- Log data transfer by HTTP(S), e-Mail, FTP(S), secure TCP, MQTT or SMS
- Camera picture transfer by HTTP(S), e-Mail, FTP(S), secure TCP or MQTT
- Remote FW-upgrade & Configuration update by HTTP(S), secure TCP or MQTT
- Internal voltage convertor for supplying 12 VDC power to the connected sensor(s),
- Stable excitation voltage to power Wheatstone bridged sensors (**ML-2013 only**),
- Firmware upgrade over the air for adding new features to your device.
- Remote configuration over the air, for adjusting your configuration from remote.

1.1 Models and Editions


1.1.1 ML-2013

The ML-2013 data logger is a small, ultra-low power, high-end data logger with built-in QUAD-band GPRS-modem. This small data logger, is further provided with an internal temperature sensor, 4GB micro SD card and an 2FF SIM card slot. The logger can be powered by an internal 3.6 Volt Lithium battery that will last for years when the logger is configured in a low-power mode. It is also possible to power the data logger using an optional integrated 3xAA NiMH solar panel.

The data logger can acquire physical signals by 4 current loop inputs, 4 digital inputs and 2 hires amplified differential voltage inputs, which can be used to connect pyranometers or in combination with a stable excitation voltage to connect “Wheatstone resistive bridge sensors” like load cells. The data logger is provided with generic serial port drivers to capture measurements from ASCII, MODBUS, NMEA or SDI-12 transponders, custom drivers can be developed on request. External sensors/transponders can be powered by the data logger itself, to prevent them to consume power while the data logger is a sleep. The excitation voltage is switched off during sleep as well. Up to 8 mathematical channels are available to calculate meaningful engineering values derived from sensed values (e.g. a polynomial to calculate a flow from a stream level).

SKU	Description
ML-2013	Powered from a 3.6V DC SAFT LSH20 or equivalent D-size lithium battery.
ML-2013-DC	With integrated 3 x AA NiMH charger powered from external 8..30V DC source.
ML-2013-PV	With integrated 3 x AA NiMH charger powered from 1Wp integrated solar panel.
ML-2013-TFT	Like ML-2013-DC but with TFT display integrated in cover.

The data logger will be supplied without pre-mounted cable glands, giving the user the freedom to choose the number and size of the glands them self to avoid unnecessary points of risk for moisture penetration. We recommend removing the PCB before drilling.

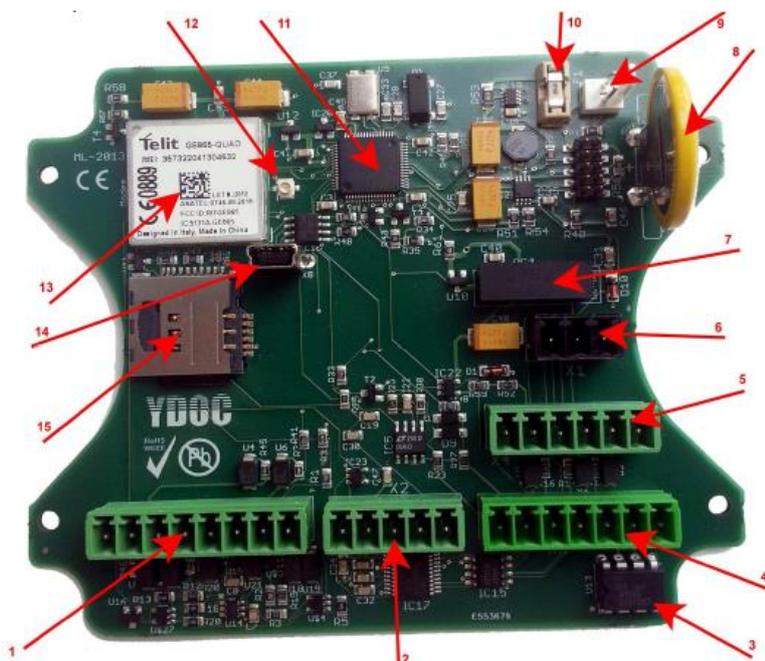

- 1) Analog inputs
- 2) RS232 connector
- 3) Excitation DC/DC convertor
- 4) Digital inputs
- 5) SDI-12, power switch and Excitation connector
- 6) RS485 connector
- 7) Power switch DC/DC convertor
- 8) RTC clock battery
- 9) Power supply connector (to cover)
- 10) Fuse
- 11) Processor
- 12) Antenna Connector
- 13) Quad Band Modem
- 14) USB Connector
- 15) SIM (2FF) & SD-card Holder.

1.1.2 ML-x15

The ML-x15 data logger is a small, ultra-low power, cost effective data logger with built-in cellular modem available for the EMEA, APAC and NA regions. This small data logger, is further provided with an internal temperature sensor, 4GB micro SD card and an 2FF SIM card slot. The logger can be powered by an internal 3.6 Volt Lithium battery that will last for years when the logger is configured in a low-power mode. It is also possible to power the data logger using an optional integrated 3xAA NiMH PV-panel or 8..30V external DC source.

The data logger can acquire physical signals by 2 current loop inputs, 3 voltage inputs (1 potentiometer input) and 3 digital inputs. The data logger is provided with one serial port to capture measurements from ASCII, MODBUS, NMEA or SDI-12 compatible sensors. External sensors can be powered by the data logger itself, to prevent them to consume power while the data logger is a sleep. Up to 8 mathematical channels are available to calculate meaningful engineering values derived from sensor input values (e.g. a polynomial to calculate a flow from a stream level).

SKU Table ML-x15		
SKU format:	ML-x15y-z (x=Modem, y=Edition, z=Power supply)	
Modem	Description	
ML-215y-z	With built in 2G cellular modem (Quad band GPRS)	
ML-315y-z	With built in 3G cellular modem (900/2100MHz UMTS/HSPA, EMEA/APAC)	
ML-N315y-z	With built in 3G cellular modem (850/1900Mhz UMTS/HSPA, North America)	
Edition	Description	Remarks
ML-x15TFT-z	With 5 analog & 3 digital inputs, serial port & TFT-display cover on accessory port.	
ML-x15ADS-z	With 5 analog & 3 digital inputs, serial & accessory port.	
ML-x15AD-z	With 5 analog & 3 digital inputs (no serial port, no accessory port).	
ML-x15DS-z	With 3 digital inputs & serial port (no analog inputs, no accessory port).	
Power supply	Description	
ML-x15y-LI	Powered from a single 3.6V DC SAFT LSH20 or equivalent D-size lithium battery.	
ML-x15y-3LI	Powered from 3x 3.6V DC SAFT LSH20 or equivalent D-size lithium batteries.	
ML-x15y-DC	With integrated 3 x AA NiMH charger powered from external 8..28V DC source.	
ML-x15y-PV	With integrated 3 x AA NiMH charger powered from 1Wp integrated solar panel.	

Example: **ML-315ADS-PV** is a data logger with built in 900/2100MHz 3G modem with PV-cover, digital & analog inputs, a serial and accessory port.

The data logger will be supplied without pre-mounted cable glands, giving the user the freedom to choose the number and size of the glands them self to avoid unnecessary points of risk for moisture penetration. We recommend removing the PCB before drilling.



- 1) Analog inputs
- 2) RS232/RS-485/SDI-12 connector
- 3) Digital inputs
- 4) 12V Power switch and alarm output
- 5) Accessory port (TFT, CAM, BT4.0, etc.)
- 6) Cellular MODEM
- 7) Internal/External antenna selection jumper
- 8) U.FL connector for external antenna
- 9) Internal antenna
- 10) Connector for optional external waterproof USB connector
- 11) Internal USB connector
- 12) Processor
- 13) SIM (2FF) & SD-card Holder
- 14) Fuse
- 15) 3V6 power supply connector (to PV or DC cover)
- 16) D-Size 3.7V Lithium battery holder (ML-x15y-LI only)
- 17) RTC clock battery.

1.2 ML-x17


The ML-x17 data logger is a small, ultra-low power, cost effective data logger with built-in 2G/3G/4G cellular modem available for the EMEA, APAC and NA regions. This small data logger, is the same as mlx-15, with the addition of an option port for expansion of possibilities.

The data logger can acquire physical signals by 2 current loop inputs, 3 voltage inputs (1 potentiometer input) and 3 digital inputs. The data logger is provided with one serial port to capture measurements from ASCII, MODBUS, NMEA or SDI-12 compatible sensors. External sensors can be powered by the data logger itself, to prevent them to consume power while the data logger is a sleep. Up to 8 mathematical channels are available to calculate meaningful engineering values derived from sensor input values (e.g. a polynomial to calculate a flow from a stream level).

SKU Table ML-x17		
SKU format:	ML-x17y-z (x=Modem, y=Edition, z=Power supply)	
Modem	Description	
ML-217y-z	With built in 2G cellular modem (Quad band GPRS)	
ML-317y-z	With built in global 3G modem (Penta band & Quad band GPRS fallback)	
ML-417y-z	With built in global 4G modem (LTE-M & Quad band GPRS fallback)	
Edition	Description	Remarks
ML-x17TFT-z	With 5 analog & 3 digital inputs, serial port & TFT-display cover on accessory port.	
ML-x17ADS-z	With 5 analog & 3 digital inputs, serial & accessory port.	
ML-x17AD-z	With 5 analog & 3 digital inputs (no serial port, no accessory port).	
ML-x17DS-z	With 3 digital inputs & serial port (no analog inputs, no accessory port).	
Power supply	Description	
ML-x17y-LI	Powered from a single 3.6V DC SAFT LSH20 or equivalent D-size lithium battery.	
ML-x17y-3LI	Powered from 3x 3.6V DC SAFT LSH20 or equivalent D-size lithium batteries.	
ML-x17y-DC	With integrated 3 x AA NiMH charger powered from external 8..28V DC source.	
ML-x17y-PV	With integrated 3 x AA NiMH charger powered from 1Wp integrated solar panel.	
ML-x17y-SLA	With integrated 12V lead acid/LiFePO4 battery charger for 21VOC solar panels.	

Example: **ML-317ADS-PV** is a data logger with built in 900/2100MHz 3G modem with PV-cover, digital & analog inputs, a serial and accessory port.

The data logger will be supplied without pre-mounted cable glands, giving the user the freedom to choose the number and size of the glands them self to avoid unnecessary points of risk for moisture penetration. We recommend removing the PCB before drilling.

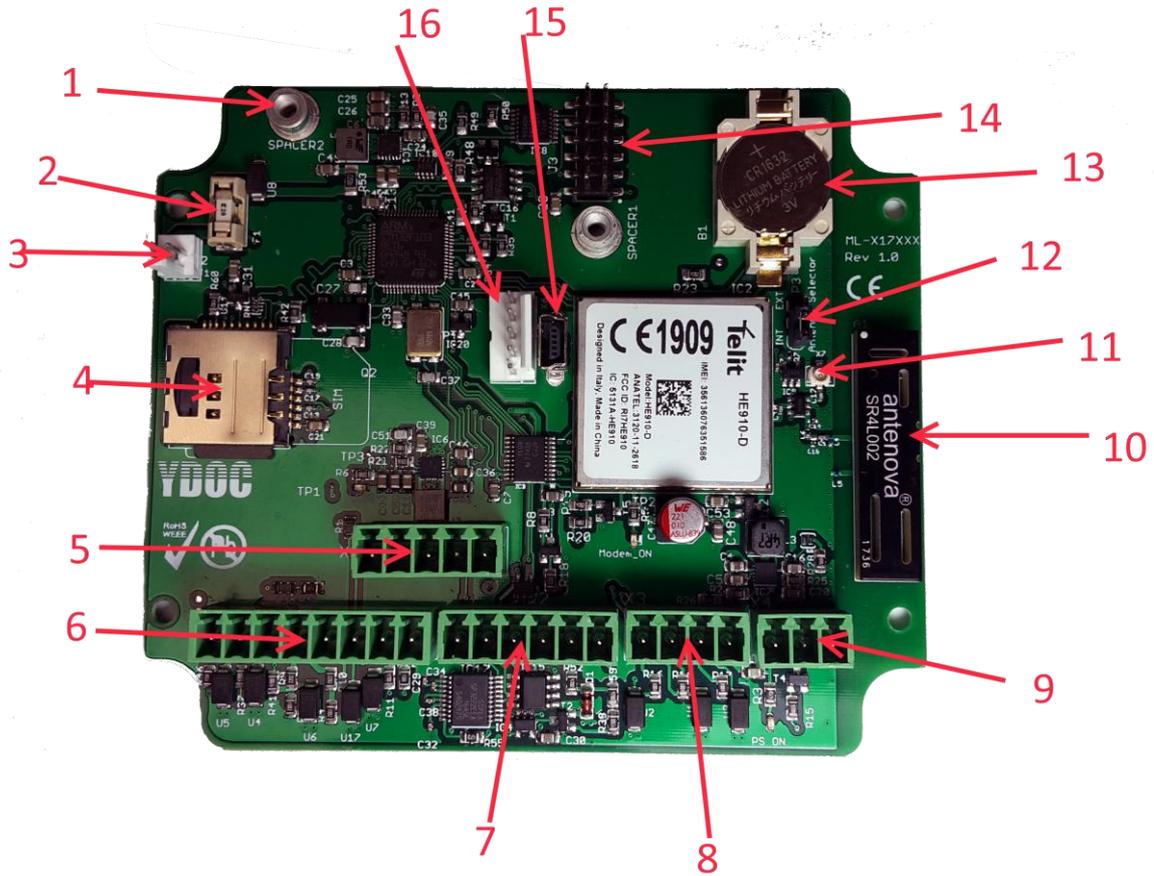

- 1) Mounting bus for option board
- 2) Main Fuse (2A Fast Acting)
- 3) 3V6 Power Supply Connector
- 4) SIM(2FF) & Micro SD-card Holder
- 5) Accessory port (TFT, CAM, etc.)
- 6) Analog input port
- 7) RS232/RS485/SDI-12 Port
- 8) Digital input port
- 9) 12 V Sensor Power Output & Alarm Output connector
- 10) Hexaband antenna for 2G/3G/4G communications
- 11) U.FL Connector for external antenna
- 12) Internal/External antenna selection jumper
- 13) RTC clock Battery
- 14) Option port
- 15) USB port
- 16) Connector for optional external IP67 USB connector


1.3 WDL-x14

The WDL-x14 is a small, battery powered, cost effective data logger with built-in cellular modem available for the EMEA, APAC and NA regions. The IP68 rated well data logger enclosure is slim enough to fit a 2" borehole and is designed to fit a www.prohydroinc.com lockable well cap. This well data logger, is further provided with a 4GB micro SD-card and an 2FF SIM-card slot. The borehole logger is powered by an internal 3.6 Volt Lithium battery (SAFT LSH20-CNR or equivalent only) that will last for years when the data logger is configured in a low power mode. The battery can be replaced by detaching the top cap, no need to remove the well data logger and sensor from the borehole.

External sensors can be powered by the data logger itself, to prevent them to consume power while the data logger is a sleep. The data logger is provided with an IP68 rated venting plug, integrated temperature and barometric sensor that can be used for compensating the readings of low cost absolute pressure level sensors. Make sure that the well cap and borehole is vented as well.

SKU Table WDL-x14		
SKU format:	WDL-x14y-z (x=Modem, y=Edition, z=Power supply)	
Modem	Description	
WDL-215y-z	With built in 2G cellular modem (Quad band GPRS)	
WDL-315y-z	With built in 3G cellular modem (900/2100MHz UMTS/HSPA, EMEA/APAC)	
WDL-N315y-z	With built in 3G cellular modem (850/1900Mhz UMTS/HSPA, North America)	
Edition	Description	Remarks
WDL-x14AD-z	With 1 digital & 4 analog inputs (no serial port).	
WDL-x14DS-z	With 1 digital input & serial port (no analog inputs).	
Power supply	Description	
WDL-x14y-LI	Powered from a 3.6V DC SAFT LSH20-CNR or equivalent D-size lithium battery.	

Example: **WDL-314AD-LI** is a well data logger with built in 900/2100MHz 3G modem with 1 digital & 4 analog inputs.

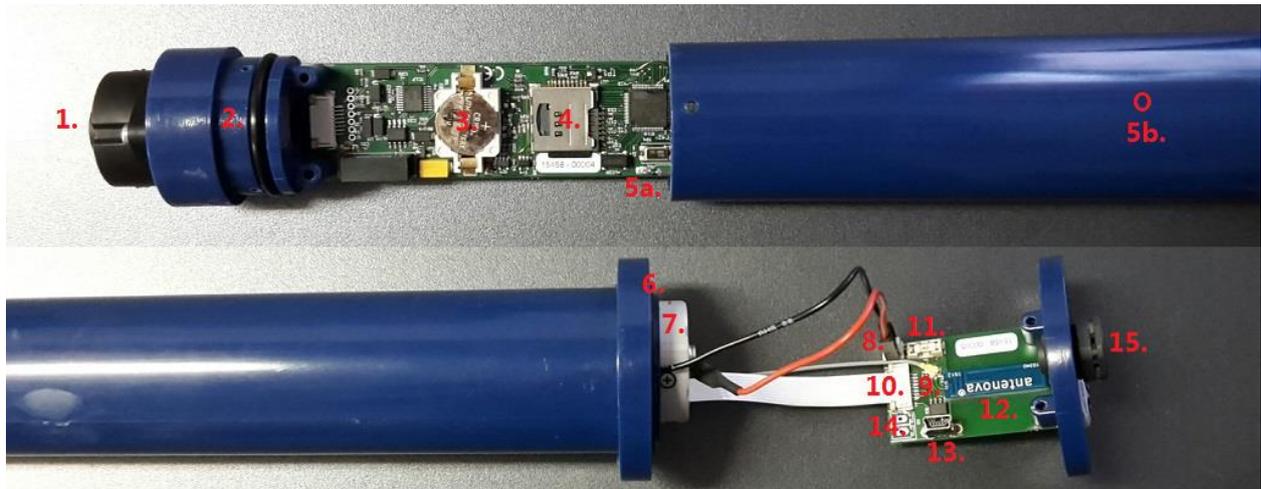

- 1) Waterproof 7-pole female Hirschmann connector (see chapter: Pin configuration)
- 2) Rubber O-ring (30x3mm NBR SHa 70)
- 3) RTC clock battery
- 4) SIM (2FF) & SD-card Holder
- 5a) Magnetic activated deployment suspension switch.
- 5b) Marker to put magnetic tape for suspending deployment (e.g. during transport)

- 6) Rubber O-ring (41x3.5mm NBR SHa 70)
- 7) SAFT LSH20-CNR 3.7V D-Size Lithium battery
- 8) 3V6 power supply connector (Max 3.7V!)
- 9) UFL connector (antenna cable to main pcb)
- 10) Flex cable connector (power and data signals to main pcb)
- 11) Fuse
- 12) Internal antenna
- 13) Internal USB connector (for local configuration)
- 14) Open collector alarm output solder pad.
- 15) IP68 venting plug

2 Getting started

2.1 Vibration

At all times the data logger must be protected against vibrations. These vibrations can harm the performance of the data logger. Especially the real-time clock can be harmed by long-lasting vibrations

2.2 Do's & Don'ts

Do's

- Always provide a dry and clean environment when you open the case of a data logger,
- When you open the case, use a Philips screwdriver of 2mm for loosening the screws,
- Protect the data logger against mechanical stress and vibrations

Don'ts

- Don't try to use a plain screwdriver for loosening the screws, you will damage the screws,
- Avoid touching the PCB directly.

2.3 Inserting the SIM-card

The wireless data functions will only work when an activated SIM, with a valid subscription is placed in the data logger. In the menu the configuration and network settings must also match to those supplied by the SIM card provider. The pin code of the SIM card must be removed prior to insertion in the data logger. To prevent problems with the SIM card it can be inserted in a mobile phone or 2G/3G data modem. In a Mobile phone or 2G/3G modem the 2G/3G, SMS and GSM data functionality can be tested.

When you have obtained a 2FF SIM-card, you can insert it into the SIM-card-holder.



Beware:

- Remove the PIN code (this can be done with the use of a mobile phone),
- Check the settings of your mobile provider,
- Check the settings for communicating via HTTP, FTP, E-mail or TCP,
- Check the capability of data communication for your service-provider,
- Make sure the SIM-card is installed correctly, and not upside down. The Oblique side of the card should be visible. (see picture).
- Installation of the SIM card needs to be done in a clean and dry environment.
- Avoid contact with the electronic parts around the SIM card.
- Remove power before changing or inserting a SIM card.
- The same applies to the SD-card.





ESD Attention: Although the data logger is designed to withstand certain amounts of electrostatic discharge, it is advised to avoid discharged risks. Especially when the housing is open and the electronic parts are exposed. Please do not touch the PCB if you don't have to. It is strongly recommended to use an earthed wrist-band when touching the PCB.

The data logger must be handled with care and never exposed to ESD discharges. When installing a sensor or other wiring, make sure there is no power on both devices. ESD discharges could cause invisible damage. This endangers long term stability and proper operation.

2.4 Power on for the First time

In the factory the data logger is programmed with the necessary system information. This information is viewable in the menu. The data logger is ready to use out of the box if the preparations are checked.

- SIM card is inserted,
- SD-card is inserted,
- Internal battery, or mains power is connected
- Antenna is connected.

Next, connect your sensors, please consult your sensor's manual for wiring.

2.5 Connect to a PC

OS compatibility: The data logger can be connected to any PC with USB 2.0 running on Microsoft Windows XP, W7, W8 or W10. The USB virtual COM-port driver is installed when installing 'YDOC-terminal'. 'YDOC-terminal' can be downloaded from www.your-data-our-care.com

3 Operating Basics

3.1 Configuration menu

The data logger can be configured by means of terminal emulation software like 'hyper terminal'. Our own terminal emulation software 'YDOC-terminal' can be downloaded from www.your-data-our-care.com or ydocTerminal for Android from the 'Google PlayStore'.

The menu is comprehensive and easy to use. For each different sensor the same approach is used. Below, one example is given to fully understand the operation of the menu. The example takes you through a configuration from start to final stage. Only a few menu-items are used in this example, for a complete overview of all menu-items, see chapter Reference. All menu items use the same approach which is explained in this example. This example explains only the configuration of the firmware, NOT the wiring. For wiring information see the reference.

Example:

Let's Configure an ML-315ADS for operation with the following:

- Analog pressure transmitter 4 .. 20mA
- CT2X conductivity / temperature sensor (INW)
- FTP data output
- EMAIL data output

Connect the logger to a free USB port on your computer and open with a terminal emulator the virtual COM-port (e.g. COM7) as assigned by Windows to the logger. The first time Windows will ask (if not already installed) for an USB-driver, which can be installed by installing 'YDOC-Terminal'.

When the terminal emulator has opened the COM-port, press:
<Ctrl>A<Shift>M<Ctrl>D to enter the configuration menu.

You'll see a screen similar to this:

Running
Configuration Menu ML-317 Logger Version 3.5 Build 4

```

Configuration Menu ML-317 Logger Version 3.5 Build 4
[0] Run
[1] Date & time          >> 2015/11/26 09:11:28
[2] System information  >> 5159422
[3] Configuration setup >>
[4] Parameter overview >> 3
[5] Maintenance
[6] Set USB password
>
    
```

First we like to give this data logger appropriate identification codes. So, press 3 <Configuration Setup>



(To avoid unauthorized local access we recommend to specify a local USB password).

You'll see this screen:

First Rename your Device by
Selecting option 1
(General Settings)

```

Configuration setup
[0] Exit
[1] General settings      >> YDOO
[2] Modem settings
[3] NTP time update      >> Not used
[4] Alarm messages      >> Not used
[5] Option boards       >> None
[6] Internal sensors    >> Not used
[7] Analog inputs       >> Not used
[8] Digital inputs      >> Not used
[9] Network signal sensor >> Not used
[A] Serial port         >> Not used
[B] Accessory port     >> Not used
[C] Derived channels    >> Not used
[D] DTU connection     >> Not used
[E] Email output        >> Not used
[F] FTP output          >> Not used
[G] TCP output          >> Not used
[H] HTTP output         >> Not used
[I] MQTT output         >> Not used
>
    
```

After selecting "General Settings" the screen will look like this:

```

General settings
[0] Exit
[1] System name          >> YDOO
[2] Data log interval    >> 00:10:00
[3] Timestamp round down >> 00:01:00
[4] Continuous alarm sampling >> Off
[5] Direct data output on data alarm >> Off
[6] Alarm output port    >> Disabled
[7] Deployment date and time >> 2015/08/31 06:55:23
[8] Daily operating time slot >> 24 hour
[9] Time zone            >> 0
[A] Summer time (daylight saving) >> Not used
>
    
```

< General

settings>

1. Press 1 and enter the name of your preference
2. Choose your data logging interval. We used 10 minutes, and NO Alarming.
3. Enter the deployment date & time. This can be a time in the future when the logger should start working. We will use the actual date & time to start right away.
4. Exit and save changes.
5. Now, the overall configuration is setup and we proceed with the configuration of the sensors and data output.

Next type 7 for Analog inputs

```

Analog inputs

[0] Exit
[1] Port 1 (mA) >> Analog
[2] Port 2 (mA) >> Not used
[3] Port 3 (V) >> Not used
[4] Port 4 (V) >> Not used
[5] Potentiometer >> Potentio
[7] Analog input test >> Not done
>
    
```

Choose 1 for Port 1 (mA) and the next screen will appear:

```

Analog input

[0] Exit
[1] Name >> Analog
[2] Sensor power switch >> Disabled
[3] Sample interval >> Data log interval
[4] Port mode >> Port 1: 4-20 mA
[5] Parameter settings >> Analog
[6] Parameter value at 4 mA >> 0 units
[7] Parameter value at 20 mA >> 100 units
[8] Determine linear conversion function (2 calibration points)
[9] Determine linear offset only (1 calibration point)
[R] Remove
>
    
```

Assign a name to the sensor (option 1: Name)

1. Set the power switch to enabled and enter the warm-up time. (the power switch will supply the sensor with 12 Volts, and will be activated the time you specify, before a measurement is taken)
2. At default Set the sample interval to the 'Data log interval' so only one sample per data log interval will be taken. You can set the sample interval to a specific value in case you want to record periodic averages (e.g. a 10-minute wind direction, see chapter: Aggregation channels) or continues alarm sampling.
3. Set the parameter name.
4. Set both minimum (option 6) and maximum (option 7) values of your sensor at 4mA and at 20mA. If you don't know those values, you could determine the scaling by measuring two calibration points (option 8). Those calibration points don't have to be at the sensors absolute minimum and maximum, but just two different points within the range of the sensor. (e.g. a measurement at 1m water level and a measurement at 2m water level, while the sensors range is 0...10m)
5. If necessary option 9 can be used to perform an offset correction by measuring a single calibration point.
6. Save and Exit

Your screen will look similar to the one underneath:

```

Analog sensor

[0] Exit
[1] Name >> Water height
[2] Sensor power switch >> Enabled; Warm up 00:00:02
[3] Sample interval >> Data log interval
[4] Port mode >> Port 1; 4-20 mA
[5] Parameter settings >> Analog
[6] Parameter value at 4 mA >> 0 meter
[7] Parameter value at 20 mA >> 10 meter
[8] Determine linear conversion function (2 calibration points)
[9] Determine linear offset only (1 calibration point)
[R] Remove
>

```

Now we add the CT2X to the system:

Before we can do this, we need to know the MODBUS address and register address of this sensor, always consult the manual of your sensor first. In this case the address of the sensor is #1. This sensor measures two parameters: Temperature and conductivity. So, we need to look up two register addresses. (Temperature: 62592 and Conductivity 62594, baud rate 38400)

Go to menu-option A <serial port 1> => RS 485 sensors.
After configuring your screen should look like this:

```

MODBUS sensor

[0] Exit
[1] Name >> MODBUS INW CT2X
[2] Port settings >> RS485 8N1; 38400 Baud; Address 1
[3] Sensor power switch >> Enabled; Warm up 00:00:01
[4] Sample interval >> Data log interval
[5] Protocol type >> RTU
[6] Start command >> Not used
[7] Ready status >> Not used
[8] Ready after >> Not used
[9] Register type >> Holding
[A] Start register >> 62592
[B] Data type >> WORD (unsigned 2 bytes)
[C] Parameter 1 >> Water temperature
[D] Parameter 2 >> Conductivity
[E] Parameter 3 >> Not used
[F] Parameter 4 >> Not used
[G] Parameter 5 >> Not used
[H] Parameter 6 >> Not used
[I] Parameter 7 >> Not used
[M] More parameters >> Not used
[R] Remove
>

```

The parameters are always read from Register start address onwards, so the specific address (62594) of the conductivity-measurement is not used in the configuration. It automatically increases the register-address in order to read it. All you have to do is select how many parameters are used, and the data type. More on this topic is included in the reference chapter of this manual.

Multiple CT2X sensors can be connected to an RS485 bus so you need to specify its address (assuming 1 in this example). This sensor is a multiple parameter sensor, so please specify which you want to log.

Attention:



Because this is a digital sensor, it takes a little bit more time to measure than an analog sensor. So don't set the sample interval of digital sensors too short. 1 second is possible, but probably not ¼ sec. Just to be sure we choose to sample at the data log interval. Consult the manual of your digital sensor and check the response time. The sample-interval must be larger than the response time of the sensor.

Next thing is the setup of the data outputs.

Before that, we have to configure the general modem settings for GPRS operation. Consult your GPRS-provider for the correct local settings. In the reference, a table is included with some international GPRS-providers and their settings. These settings might have been changed.

Go to Menu-option 2 <Modem settings>

```

Modem settings

[0] Exit
[1] Provider selection
[2] Network          >> 3G+2G fallback
[3] APN access point >>
[4] APN username    >>
[5] APN password    >>
[6] APN authentication >> PAP (plain)
[7] Network signal test >> Not done
[8] APN login test  >> Not done
>
    
```

The meaning of this menu-option is to configure the settings of your provider. For the right settings, please consult your local provider. After this configuration it is advised to check the connectivity of your device, by using the APN login test. After correct configuring it should look like this:

```

APN test

Modem full power
Please wait...
ATED;+CMEE=2;+CCLK="15/11/26,14:26:21+00";+CFUN=5;+CPIN?
+CPIN: READY
OK
AT+CREG=2;+CREG?
+CREG: 2,1,"17F2","0A5C825",2
OK
Registered on 3G network
ATS12=20;#DST0=1;+CGDCONT=1,"IP","internet";#SGACTCFG=1,5,180,1
OK
AT#SGACT?
#SGACT: 1,0
OK
AT#SGACT=1,1,"xs4all","****"
OK
#SGACT: 10.137.12.103
Modem idle

APN test OK

Press any key! >
    
```

Now we can setup the FTP, TCP and Email output

Therefore, go to menu-option:

- E Email output
- F FTP output.
- G TCP output
- H HTTP output

Enter your server-settings.

It should look like this:

Email settings

```

[0] Exit
[1] Name >> Email
[2] Send interval >> Normal 01:00:00; Alarm Not Used
[3] Send delay >> Not Used
[4] SMTP Server >> smtp.provider.com
[5] SMTP Port >> 25
[6] User name >> rehla01
[7] Password >> *****
[8] Originator address >> r.kleine@provider.com
[9] Destination address >> your@provider.com
[A] Subject >> YDUC upper stream
[B] Data Format >> Native (txt)
[R] Remove
[T] EMAIL test >> Not Done
>
    
```

Beware:
Some providers
strictly check
the Originator
address. So
make sure this
address is valid.

Now perform an Email test and check if it is working right.

It is strongly recommended to include some internal sensors in the configuration, because of the monitoring of the performance of the data logger itself. Most users like to keep track of the battery-life for example.

Go To menu-option 6 <internal sensors>

```

Internal sensors

[0] Exit
[1] Name >> Internal
[2] Sample interval >> Data log interval
[3] Battery capacity >> 14000 mAh
[4] Battery replaced >> Yes
[5] Rest capacity >> Not used
[6] Rest power >> Not used
[7] Processor temperature >> Processor temperature
[8] Average voltage >> Not used
[9] Max voltage >> Not used
[A] Min voltage >> Min voltage
[B] Average current >> Not used
[C] Max current >> Not used
[D] Min current >> Not used
[E] Operating cycle >> Operating cycle
[F] Free disk space >> Not used
[R] Remove
>
    
```

A sample interval of 1 second is fine. All internal sensors are very fast.
 Set the "Battery Replaced" to "Yes", only when you installed a new lithium battery.
 Select the items you like to be informed about.
 See the reference for a complete description of the items.

Now your data logger is configured and ready to use.
 To check your wiring and sensors, you can evaluate the actual values.
 To see them press: <Ctrl>A<Shift>V<Ctrl>D

The result should be like this:

13/07/05 14:22:04 Actual Values ML-315 Logger Version 2.1 Build 2			
AIN1	Waterlevel	-25	meters MSL
TMP	Temperature	20.2	C
PRS	Pressure	0.2	psi
RCi	Rest Capacity	100	%
PTi	Processor Temperature	57.4	C
Vi	Voltage	3.6	V
Ci	Current	82	mA

4 Reference

4.1 Principle of Operation

4.1.1 Intervals

Your YDOC data logger is capable of collecting and storing data of multiple sensors. To accomplish this, many tasks are performed. These “tasks” are scheduled and executed on their specified time. The timing of this process is very important and is determined by the internal scheduler. This scheduler keeps track of all the internal states of the various tasks and assigns processor time to the different tasks. Each task is executed on its own interval. To understand more about this, First we explain the different intervals.

There are three different intervals:

- 1) Sample Interval
- 2) Data Log Interval
- 3) Send Interval

4.1.1.1 Sample interval

The sample interval is the interval at which a sample from the sensor is taken (**expected**). So, measurements from sensors are done at the sample interval. The sample interval is valid **ONLY** when the device is in the active state. When the data logger is in sleep-mode, the tasks, triggered by the sample interval will **NOT** execute, unless they are used in aggregations (e.g. a 10-minute average, see chapter Aggregation channels), scheduled for continuous alarm sampling, or if a pending alarm is detected and you have set “alarm set delay” to number of samples”. So, in most cases you could follow the default data log interval to take a sample.

4.1.1.2 Data logging interval

This interval determines when a data value, obtained by the sample interval-task, is stored onto the SD-card. This type of interval is **ALWAYS** valid. So, even when the data logger is in sleep-mode, it will wake up when the Data logging Interval has reached its count.

4.1.1.3 Send Interval

The send interval determines the interval on which data is send, via the internal modem. This interval is **ALWAYS** valid, even if the data logger is in sleep-mode.

4.1.1.4 Example

Let's evaluate the following settings of the data logger:

- Sample Interval: 5 seconds
- Data Log Interval: 10 minutes
- Send Interval: 3 hours

When the configuration is ready, and the user disconnects the USB-Cable;

1. Data logger is switched into sleep-mode, and current draw is reduced to a minimum level.

2. The Sample interval of 5 seconds is discarded (except for special alarming modes), because this interval is only active when the data logger is NOT in sleep-mode. So, nothing happens until the Data Log interval has reached his count. (So, this happens on 0, 10, 20, 30, 40, 50 minutes every hour)
3. When the Data Log Interval count has reached his count, the data logger will awake from the sleep mode, and will take a sample and stores the data on the SD-card. When the sample is taken, the data logger goes into sleep-mode again. This is repeated, until the time has matched the Send interval. So, in this example, this is 3 hours.
4. When Data Send interval is reached, the data logger will wake-up, and starts to send the previously collected data (stored on the SD-card) to the server. So, in this example, every 10 minutes a sample is taken, and every 3 hours, 18 samples are send.

Note: So, the data logger does not perform any averaging. Even if the sample interval is much faster than the data log interval, only one sample is stored.

The use of the sample interval is for evaluating proper behavior of the system, while the USB is connected, and for special alarming modes. Because in that case, the sample interval is valid, and the user can observe the value's obtained from the sensor in real time. In this case, the user can evaluate these values every 5 seconds.

4.1.2 Common data output settings

Data can be transferred by various internet protocols a/o FTP & MQTT of which the specific settings are described in individual chapters. They however share some protocol independent features that are describe below.

4.1.2.1 Send delay

Data output transmissions will be performed at scheduled discrete intervals. Setting-up a cellular connection takes some time, which is normally more than enough to acquire measurements scheduled at the same moment. If acquiring a sample from a slow sensor or when taking a hires camera picture, it might not be ready in time to be included in the current transmission. Specifying a few seconds of send delay might avoid this to happen. A send delay could also be applied to avoid overload on a constraint server due to simultaneous transmissions of a lot of units.

4.1.2.2 Output type

Per output driver you can specify which type of data you want to output: 1) All logged data since the previous successful transmission, 2) Just the last know sampled actual values or 3) a heartbeat message.

The primary output is normally chosen for transmission of the logged data.

A heartbeat can be used to indicate thru an alternate output that a system is still a live or to have an entry point in time to do a remote configuration if not possible thru the primary output (see: chapters remote configuration).

4.1.2.3 Data format

This defines the data format of the transmitted content/file. This can be our native TXT format, JSON or a CSV (comma separated value) format which can easily be picked up by third party applications like Microsoft Excel. The column order of the CSV file, follows the order of the parameter list (see: chapter "Parameter overview"). We prefer native or JSON format as it can contain data as well is diagnostic info.

4.1.2.4 Data filter

The logger records Log Data (measurements) as well as system Diagnostics. With a data filter you can specify which you want (or both) to include in the transmission.

4.2 Parameters

All through the configuration-settings of the data logger, you will encounter parameters to setup your logger. They are used on all ports (analog, digital, serial) and are generic in use. This section describes the use and properties of parameters. Below a screenshot of some parameter-settings are shown.

```

Parameter Settings

[0] Exit
[1] Name                >> Analog
[2] Code                >> AIN
[3] Unit                >> meter
[4] Value factor        >> 1
[5] Value offset        >> 0
[6] Decimals            >> 3
[7] Data log            >> 0n
[-] Data transpond      >> Disabled
[-] Alarm message       >> Disabled
[A] Alarm log           >> 0n
[-] Alarm output        >> Disabled
[C] Low-low limit       >> N/A
[D] Low limit           >> N/A
[E] High limit          >> N/A
[F] High-high limit     >> N/A
[G] Alarm set delay     >> 0 samples
[H] Alarm reset hysteresis >> 0.5 meter
[R] Remove
>

```

4.2.1 Name

A appropriate name for the parameter (real life measurement).

4.2.2 Code

A short alphanumeric code to designate the parameter. This code will be used in the data files.

4.2.3 Unit

The unit of the real-life parameter (i.e. meters)

4.2.4 Value factor

Multiplier to transform the electrical signal into a real-life value. Default is 1. So, when the value factor is 2, all measurements are multiplied by 2. (in math: $F(x) = ax+b$, where a equals the value factor)

4.2.5 Value offset

Also to transform the electrical signal into a real life value, but now an addition (+) default = 0. (in math: $f(x) = ax+b$, where b equals value offset) This is very convenient while using 4..20 mA sensor, because they introduce an offset. (4 mA = 0 centimeter)

4.2.6 Decimals

The numeric precision of the value, displayed and stored on the SD card. (of course, not the real-life precision, only the numeric presentation)

4.2.7 Data log

Setting which enables the storage of the parameter to the SD card. When set to off it will be measured and displayed, but NOT stored on the SD card. Default set to "ON".

4.2.8 Data transpond

It's only enabled if you have installed a Radio or Satellite modem. If you want this parameter to be transmitted by the Radio or the Satellite modem, put it to "ON".

4.2.9 Alarm message

Here, the user can select whether he wants to receive an alarm message on this parameter (in alarming conditions) or not. Alarm messages are send by SMS, e-Mail or MQTT.

4.2.10 Alarm log

Setting which enables the storage of the alarm condition of the parameter to the SD card. When set to on it will store an unscheduled data log in a single data record, and the passing of the alarm limits in a system record.

4.2.11 Alarm output

Setting which sets or clears the digital alarm output port when the selected alarm limit is passed (Low, High or both).

4.2.12 Alarm limits and delays

Within every parameter settings menu, the user can define all limits and delays to customize his alarming mode. More info on these settings and the alarming mode is found in section: [Alarming](#)

4.3 Configuration Menu Settings

This Chapter describes the details of the configuration-settings of your data logger. The configuration menu is entered by using YDOC-terminal and typing <Ctrl>A<Shift>M<Ctrl>D.

4.3.1 Date & Time

This section allows you to set date and time manually. If pressed enter, the existing system data/time is displayed.

4.3.2 System Information

A read only menu-section which displays all specific details about the data logger, an example is given below:

```

System Information ML-315 Logger Version 2.2 Build 1

[0] Exit
[-] Serial number          >> 5024367
[-] Hardware model        >> ML-315
[-] Modem type            >> UMTS UL865-EUR
[-] IMEI number           >> 355856050243670
[-] Hardware edition      >> ADS (Analog+Digital+Serial)
[-] Production date       >> 2015/06/22
[-] Test date             >> 2015/06/23
[-] RTC adjustment frequency >> 512.0115 Hz
[-] Low power sleep current >> 0.09 mA
[-] Analog input 1        >> Span = 1.098; Offset = -1
[-] Analog input 2        >> Span = 1.102; Offset = -1
[-] Analog input 3        >> Span = 1.053; Offset = -1
[-] Analog input 4        >> Span = 1.056; Offset = -1
>
    
```

4.4 Configuration Setup

This menu-section allows you to configure your data logger for your specific task. This section is divided into logical items, which contains more settings will be discussed next: Below a screenshot of the configuration setup is displayed:

```

Configuration setup

[0] Exit
[1] General settings      >>
[2] Modem settings
[3] NTP time update      >> Not used
[4] Alarm messages      >> Not used
[5] Option boards       >> None
[6] Internal sensors    >> Internal
[7] Analog sensors     >> Water height; Potentiometer
[8] Digital sensors    >> Display
[9] Network signal sensor >> Not used
[A] Serial port        >> Not used
[B] Accessory port     >> Display
[C] Derived channels   >> Used
[D] DTU connection    >> Not used
[E] Email output       >> Not used
[F] FTP output         >> Not used
[G] TCP output         >> Not used
[H] HTTP output        >> Not used
[I] MQTT output        >> Not used
[J] SMS output         >> Not used

>
    
```

Each item is explained below, including sub items

```

General settings

[0] Exit
[1] System name          >>
[2] Data log interval   >> 01:00:00
[3] Timestamp round down >> Not used
[4] Continuous alarm sampling >> Off
[5] Direct data output on data alarm >> Off
[6] Alarm output port   >> Disabled
[7] Battery protection >> Default
[8] Permanent SD storage >> Data & Diagnostics
[9] Deployment date and time >> 2018/04/26 12:19:47
[A] Daily operating time slot >> 24 hour
[B] Daily schedule time shift >> Not used
[C] Time zone           >> 0
[D] Summer time (daylight saving) >> Not used

>
    
```

4.5 General Settings

Here you enter your global settings, like datalog interval etc. These are the settings:

4.5.1 Exit

Exits the menu

4.5.2 System Name

Allows the user to give a name to the data logger (up to 32 characters). This name will be used in the data files, produced by the logger.

4.5.3 Data log interval

This is the interval on which the logger will write a measurement to its SD-card. These records will be present in the data file and this setting defines the size of the data file per interval. The data log interval knows 2 different modes:

4.5.3.1 Normal mode

Normal data logging mode, the regular data will be logged



The normal interval must be greater than the alarm interval and can't be greater than the smallest normal send interval and can't be smaller than the highest normal sample interval

4.5.3.2 Alarm mode

Alarm mode data log interval defines the (often faster) rate of data logging, during alarming conditions



The alarm interval must be less than the normal interval and can't be greater than the smallest alarm send interval and can't be smaller than the highest alarm sample interval

4.5.4 Timestamp round down

This feature allows you to round down the timestamps in the data log to fixed time brackets. Some sensors will take a few seconds to finish data reading, and as a result you get timestamps like 12:50:07. If you want to round it down to 12:50:00, you can set the round down to 10 seconds.

4.5.5 Continuous Alarm Sampling

This is an advanced feature that allows the user to act fast on exceptional situations, while the normal data log interval is slow. This setting introduces a second interval, which must be faster than the normal data log interval. First read the basics of the [alarming interval](#). Normally, the alarming-mode can only be entered by awaiting the data log interval, but this (global) setting allows the user to define a faster interval. The logger will now wake on this faster interval, but not store the data. It must be enabled in the parameter-settings by means of setting alarming conditions. Only a Sensor with a parameter with alarming conditions is sampled with his defined sample interval.

Example:

A user has chosen a data log (normal) interval of 10 minutes. The temperature-sensor must NOT get above 25 degrees. When the temperature reaches the limit, it takes the logger up to 10 minutes, before it gets into the alarming mode (with a faster alarming interval, of course). Now, the continuous alarming mode, changes this. When the sample interval of concerned sensor is set to i.e. 1 minute, the data logger will wake every minute, and take a measurement, but NOT store this on the SD Card. So, the user ends up with a normal data file, with every 10 minutes a new data record, and the system is responding within 1-minute max. on an alarm situation.

4.5.6 Alarm output port

The “Alarm output port” can be used to “switch on” or “trigger” an external device in case of an alarm situation by means of an [“open collector output”](#) (ML-x15/WDL-x14) or the “module power switch” (ML-2013). When in “Continuous state” the output will be activated as long as an alarm situation exists. If you only want to trigger an external device when a new alarm situation occurs, you can specify a “One-time pulse” with a certain pulse width in seconds. If you want to re-trigger the external device at every sample interval, while in alarm, choose “Repeating pulse”.

Alarm output port

```

[[0]] Exit
[[1]] Disabled
[[2]] Continuous state
[[3]] One-time pulse
[[4]] Repeating pulse
>Pulse width (sec):
    
```

Note: When a logger is awake (e.g. during USB connection) and frequently sampling its sensors and inputs then “repeating pulse” may look similar to “continuous state”, due to overlapping pulses.

4.5.7 Battery protection

Choose ‘Rechargeable batteries’ when NiMH batteries are inserted. In this mode the data logger will not start if the voltage is below 3.4V, giving a DC-source (e.g. solar panel) the chance to sufficiently replenish a depleted battery.

Choose ‘Lithium batteries’ when primary batteries are used, this will prevent the batteries to be drained while connected to USB by going in to low-power sleep after 3 minutes of non-activity.

4.5.8 Deployment Date and Time

Here you enter the specific Date & Time On which you like the measurements to start for the first time. This feature allows you to configure your data logger (in a nice and warm environment) before you install it in the field. It prevents the device to measure and send fake data, due to the dislocation of the unit. If this feature is used, the unit will sleep until the deployment date & time.

4.5.9 Daily operating time slot

This setting allows you to disable the data logger from operation, outside this interval. This makes sense when measurements are correlating with working hours or in other specific situations. E.g. a data logger won’t alarm, or log data, when the temperature of the boiler is too low, while no-one makes use of that. The logger will alarm you, when this happens during a working day.

4.5.10 Time zone

Time offset to meet local time zones (half’s and quarters are allowed).

4.5.11 Summer time

This setting allows the data logger to adjust its internal clock to summer time conventions. Worldwide, there are multiple conventions, and therefore the user can adjust it to manually. Also a couple of preprogrammed summertime conventions are selectable (Europe / USA). OR the user can disable the feature (default)



When the user enables the summertime feature, as a consequence, there will be an anomaly in the data. At the beginning and at the end of the summertime-period.

4.6 Modem Settings

This section allows the user to setup the communication with the 2G/3G network, according to the settings, received from the service provider. Please consult your service provider for the right setting, before consulting your YDOC dealer.

4.6.1 Provider Selection

This is an automated procedure which gives the user the overview of networks in the vicinity of the logger. Information about the provider and it's 2G or 3G capabilities are shown. The user can select his network of interest, or, he can set the device to automatic.

```

Provider selection

AT+COPS=3,0;+COPS?
+COPS: 0,0,"NL KPN",2
AT+COPS=?
+COPS: (2,"NL KPN",20408), (2,"NL KPN",20408), (1,"T-Mobile
NL",20416), (1,"vodafone NL",20404), (1,"T-Mobile
NL",20416), (1,"vodafone NL",
"20404"), (0-4), (0,2)

[0] Exit
[A] Automatic selection >> 0n
[1] NL KPN (3G) >> Automatic selected
[2] NL KPN (2G) >> Automatic selected
[3] T-Mobile NL (3G)
[4] Vodafone NL (3G)
[5] T-Mobile NL (2G)
[6] Vodafone NL (2G)
[D] Deregister network
>
    
```

The use of this feature is, to let the user decide which network he will use, or automate that for him.

In cases where the logger is situated near a foreign border, it is very important to make sure that the logger won't use the foreign network. Very often there are high costs concerned with the use of a foreign network. In these cases it is best to manually select your internet network provider (ISP). It will save you a lot of costs.



All providers that are within reception area are shown, and the user can select his network of preference. The Fallback option 3G->2G is very good in areas where both are available but not that strong.

4.6.2 Access Point Name (APN)

Name of the access point that your provider has defined, consult your provider for this setting. Sometimes (when authentication is enabled) a username/password is required, else leave blank. Also consult your ISP for this.

4.6.3 APN Authentication

The protocol, used for authentication. The user can select PAP or CHAP. Please consult your ISP for the right setting. (PAP uses no encryption for the authentication and CHAP uses improved security, by using Hash algorithms.

4.6.4 Network signal test

This is no setting, but a test to check network reception. It is very convenient to check your network reception at the installation site. A logger, which is configured at the office may NOT be working fine at the installation site. So, test this first, and make sure that the reception is sufficient. (1 bar absolute minimum, 3 bars is very nice)

4.6.5 APN login test

You should test the APN login after changing some settings, in order to verify the network connection.

4.7 NTP time update

This feature enables the automatic synchronization of the internal clock, by means of a Network Time Protocol (NTP) server on the internet.

4.7.1 Time Update

Sets the feature on or off.

4.7.2 Update interval

Interval on which the time is checked by the NTP mechanism, its fixed to 24 hours.

4.7.3 Server

IP-address or URL of the NTP-server

4.7.4 NTP Port

Port of the protocol, default is well known port 123

4.7.5 Time update test

Manually forces device to update time via NTP, in order to test the feature.

4.8 Alarm messages

Alarm messages can be send as SMS, by e-mail or MQTT (you have to choose one of the drivers).

To use e-mail or MQTT you have to enable/configure the corresponding driver, see chapter "Email or MQTT output". But if you don't want to use the driver to transmit the "Log data" as well, its recommended to schedule the driver to transmit just the "Actual Values" once a day to avoid unnecessary communication payload and according power consumption.

4.8.1 System Alarm

Check this option if you want to send system alarms messages (like Deployment start, sensor timeouts (sensor could be broken), or TCP/FTP/HTTP server not available, etc.)

4.8.2 Data Alarm

Check this option if you want to send data alarms messages (e.g. when a measurement is outside its defined limits).

4.9 Option boards (ML-x17 only)

Option boards can be used to add additional inputs to an ML-x17 data logger or to perform signal conditioning. You can mechanically stack up to 3 option boards, but only one input board (OI) per category ID (CID, internal bus address). Some OI-boards are having a switch to choose a different CID, so you can stack multiple similar OI-boards. Converter boards (OC) don't have CID's and you can stack as many OC-boards as mechanical feasible. OC-boards don't make use of the internal control bus, but are wired to existing inputs/outputs/ports.

```
Option boards

[0] Exit
[1] Analog (0B1) >> ML-0I-AD-80MV
[2] Analog (0B2) >> ML-0I-AD-20MA
[4] Barometric >> None
[5] Humidity >> None
[6] Serial port >> ML-0I-COM-SDI12
>
```

This menu is to indicate which option input boards are mounted, the actual configuration of individual input parameters is performed elsewhere, depending on the type of option board. As the sensors of the barometric and humidity boards are located inside the enclosure, they will be added to the list of internal sensors.

4.9.1 Calibration

To get the best accuracy from your analog inputs we recommend to perform a two point user calibration (See chapter: Analog inputs – Determine linear conversion). When a two point calibration is not feasible due to the nature of the input source, we recommend to do a 1 point calibration (See chapter: Analog inputs – Determine linear offset) . If a one point calibration is not feasible either, please perform a zero-calibration.

4.9.2 Zero-calibration

1. Specify the correct theoretic range of your sensor (see chapter: Analog inputs - Parameter value at)
2. Disconnect your sensor
3. For single ended inputs connect the input to ground and for differential inputs short-cut the two differential inputs.
4. Perform a 1 point calibration (See chapter: Analog inputs – Determine linear offset). For the calibration point enter the expected physical value when the sensor output signal is zero. (e.g. 0W/m2 for a pyranometer).

4.10 Internal Sensors

The data logger is equipped with “internal sensors” in order to provide an insight in the status of the system. We strongly recommend using this feature, because it tells you whether a system is running OK or that a problem may arise in the near future (e.g. battery status)

4.10.1 Name

Name of this driver. Default is “internal” may be edited.

4.10.2 Sample interval

The sample interval of the internal driver. Default is same as data log interval. When a user like to have fresh data while using USB, he can adjust it to a higher rate. More on intervals see chapter: [Principle of Operation](#)

4.10.3 Battery Capacity

Used for keeping track of the remaining battery capacity. The users here define the capacity of the new battery placed.

4.10.4 Battery Replaced

The user must select this when he installs a new lithium battery. The calculations of the rest capacity will be reset (battery rest capacity 100%)

4.10.5 Rest Capacity

Remaining capacity of the lithium battery. In percentage of a full battery.

4.10.6 Rest power

Same parameter, but in mAh



Attention: the battery-full parameters are only representative when used in lithium battery-only systems. When using a solar panel or external power they won't work. Their readings are not true in this case. (this is because the battery is charged, without updating the calculations).

This is no problem, because in these systems, the battery status is of minor importance. With solar systems, keep track of the minimum battery voltage instead of rest capacity or rest power.

4.10.7 Inner Pressure

The WDL-x14 is and the ML-x17 can be provided with an internal pressure sensor ranging from 300 to 1200mBar, when the casing is provided with a venting plug the measured inner pressure will equal the atmospheric barometric pressure. When you have connected an absolute water level pressure sensor you can use a calculated channel to subtract the inner pressure from the absolute measured water level pressure to calculate the relative pressure (water column height).

4.10.8 Inner Temperature

The WDL-x14 is and the ML-x17 can be provided with an internal casing temperature sensor, this temperature is internally used for temperature compensation of the inner pressure readings.

4.10.9 Processor Temperature

Temperature of internal processor, which is related to the ambient temperature. Because the data logger is very low power, and is only awake for a short time, the processor won't get warm, and has practically the same temperature as the environment. You can use this sensor for approximation measurements. And also for diagnostic measurements.

4.10.10 Average Voltage

The voltage of the connected battery, averaged to get a real practical value

4.10.11 Max Voltage

Battery Voltage, maximum of interval

4.10.12 Min Voltage

Battery voltage, minimum value of interval. This parameter is very practical to use for diagnostic measurements. Particularly when the modem sends data, the battery voltage will drop, and must not get too low (2 Volts) This parameter is a nice quality figure for the status of the battery. When this value drops a lot, it is wise to exchange the battery, or charge it. With solar systems, in the dark months, this can be an issue, and this can be solved with the aid of good weather.

4.10.13 Average, Max, Min current

Same as above, but for current. The data-send sessions are clearly recognized by the use of these parameters.

4.10.14 Operating cycle

This virtual sensor measures the time that the data logger is awake, performing tasks. This gives also good diagnostic information. When i.e. the GSM signal is very weak, retries will occur, and the session will consume more time. This parameter provides information on the proper operation of a system. The Operating cycle is measured in seconds.

4.10.15 Free disk space

Shows the remaining disk space on the SD Card. In most cases there is sufficient space left.

4.11 Analog inputs

This section covers the settings of analog inputs (e.g. mA and V inputs)

```

Analog input

[0] Exit
[1] Name                >> Water height
[2] Sensor power switch >> Enabled; Warm up 00:00:02
[3] Sample interval    >> Data log interval
[4] Port mode          >> Port 1; 4-20 mA
[5] Parameter settings >> Analog
[6] Parameter value at 4 mA >> 0 meter
[7] Parameter value at 20 mA >> 10 meter
[8] Determine linear conversion function (2 calibration points)
[9] Determine linear offset only (1 calibration point)
[R] Remove
>

```

4.11.1 Sensor power switch

This is used to power the sensor, it converts the battery-voltage into 12 volts. Here, the user defines if the power switch is used and also the warmup time of the sensor before measurements are done. More on the power switch see chapter: [Power Switch](#)

4.11.2 Sample interval

Interval on which the sensor is measured. Normally set to data log interval.

4.11.3 Port mode

The user can select the mode of the analog input (0..20 mA or 4..20 mA or Volts (volt port))

4.11.4 Parameter settings

See chapter: [Parameters](#)

4.11.5 Parameter value at (min & max range)

Here, the user can specify the mapping between the physical values to be measured and the sensor output signal. Please specify the theoretical expected physical value at the minimum output signal of the sensor and the expected physical value at the maximum output signal (e.g. 4mA equals a level of 0m of water and 20mA equals to 10m. A linear interpolation will be performed on all values in between.

4.11.6 Determine linear conversion function (2 calibration points)

This is an automated function to help the user to set the right conversion function into the data logger. This feature will determine the same function as described above, but will use a physical readings instead of a manually entered figures. The user will be prompted to measure and enter physical values at 2 calibration points (e.g. 2 different sensor heights in a water column). This feature is convenient while performing a field calibration and no factory calibration data of the sensor is available.

4.11.7 Determine linear offset only (1 calibration point)

This features is an automated calibration function for the offset only, make sure you have first specified the theoretic correct range (see above: Parameter value at). The user will be prompted to measure and enter the physical value at 1 calibration point. This procedure is a/o convenient when you have installed a level sensor, but you don't know it's exact well depth.

4.12 Digital inputs – Pulse counter

This section describes the operation of digital inputs, NOT to be confused with serial sensors, which also is a digital technique. A digital input is an input which measures the digital value of the input signal. This is a discrete value “0” or “1”. Examples of digital sensors are: switches, rain gauges and digital pulse devices. Digital inputs have the advantage that they are not that depended on their sample rate as analog sensors are. This is because they are interrupt-driven. There are several modes of operation on a digital input: counting pulses, generating alarms, counting on-time, recording states or trigger actions.

Below, a menu of the settings of a digital pulse input is shown.

```

Digital pulse

[0] Exit
[1] Name                >> Digital pulse
[2] Sample interval    >> Data log interval
[3] Port mode          >> Port 2; Internal pull up
[4] Register mode      >> Pulse (low frequency)
[5] Units per pulse    >> 1
[6] Register value     >> 0 Pulses
[7] Register reset     >> Off
[8] Log each counter change >> Off
[9] Counter (unit)     >> Counter
[A] Quantity (unit)    >> Not used
[B] Mean rate (unit/h) >> Not used
[C] Max rate (unit/h)  >> Not used
[D] Min rate (unit/h)  >> Not used
[R] Remove
>
    
```

4.12.1 Sample interval

This is exactly the same feature as in other menu's, although there is something interesting to notice about the sample interval of a digital input (pulse sensor). With analog inputs, the sample rate defines how many times an input is sampled. So, if your sample interval is very low, you may miss some events. But with digital inputs, this is NOT the case. The digital inputs are interrupt driven, and respond immediately on an event. So, even when your sample rate for the digital input is very low, no events are missing. This is an important difference! So, what is the use of the sample interval in respect to digital inputs? It defines the update rate of the counter value connected to that port.

Example: Suppose a user connects a wind speed sensor (anemometer) to the digital input, and this sensor generates a pulse with a frequency of 13 Hz. So, every second, the sensor has generated 13 pulses. Now the sample interval was set to 5 seconds. What happens is this: The data logger will count all pulse, and update the counter value every 5 seconds. So, the user has every 5 seconds a new data value.

4.12.2 Port mode

This defines the electrical behavior of the input (pull up / pull down)

4.12.2.1 Pull up

In this mode, a resistor is connected (from the input) to the positive rail of the internal power supply. So, in order to create an event, the external device must pull the input to the ground. So, use this mode when you have a “negative switching” sensor. (a device that switches to ground and has no voltage to drive the port, e.g. a tipping bucket rain gauge)

4.12.2.2 Pull down

In this mode, a resistor is connected (from the input) to the ground of the data logger. So, in order to create an event, the external device must drive the input with a positive voltage. So, use this mode when you have a “positive switching” device. (a device that drives the data logger’s input with a voltage)

4.12.3 Register mode

Here you choose if the logger should register into the flash memory each single pulse, or units, which can consist out of hundreds of pulses. Mostly you use Pulse, because most digital sensors like rain gauge are generating at max speed 1 or a few pulses per second. If you use for instance a flow meter, or anemometer that generates multiple pulses per second, and a completed unit in a few seconds, its high frequency and you should use unit as a register mode, or else the logger could not keep up the speed to write all the individual pulses to the flash memory.

4.12.4 Units per pulse, or pulses per unit

Factor for transforming input pulses to real-life unit values. It depends on register mode setting.

4.12.5 Register value

Sometimes you like the counter to start from an existing value (perhaps the counter value of an electricity meter you just connect?) Here you enter the initial value the counter must start with. This value is updated when a pulse or unit (depends on register mode) is measured on the input, so each time you consult this menu, this setting will be accurate automatically.

4.12.6 Register Reset

User can select if he wants the counter value to be reset at midnight, or that the counter is always incrementing (32 bits).

4.12.7 Log each counter change

This is only possible with low frequency sensors. The event is logged and a timestamp is added. I.e. if you like to count the customers, visiting your store, and you like to make a nice statistical graph, this feature is convenient (you can see busy hours, slow hours etc.).

4.12.8 Counter

This is the parameter, connected to the digital input. It behaves like a normal parameter (see [Parameters](#))
Note that the counter is not directly related to the amount of pulses at the input, the value is first scaled by the “pulses per unit” or “units per pulse” factor

4.12.9 Quantity

The Quantity is the number of units occurred during the log interval. So, if you add up all Quantities, the value is the same as the counter. This is convenient with i.e. rain measurements. The counter gives you a total of all precipitation since installation (or last automatic reset), and the quantity gives you the value per log interval.

4.12.10 Mean-, Max- and Min Rate

This is the speed of increase of the counter value. When e.g. a water meter is connected. The counter contains the total pumped volume, and the rate contains the flow of the water. The unit is: units/h (in case of the water meter l/h).

4.13 Digital inputs - Alarm trigger

This feature uses the same electrical input as the previous (digital input: pulse counter), but it handles the signal differently. When the input is configured as an alarm input, instead of a pulse input, it has another menu and the purpose of the measurements is different. The difference between the pulse measurement and the alarming mode, is that with pulse measurement the change of the input signal is expected, and very often frequently, while in the alarming mode, a change in input signal is an exception. That's why you don't find functions like min, max, average. The Digital Alarm itself is not an Data Alarm, but puts the logger into alarming mode (using alarm intervals if applicable), and starts a direct measurement of all sensors trying for instance to catch data alarms, and the driver also directly logs it's changing state. If you also have put on direct data output on alarm (general settings), the logger will also start the output drivers (at both rising and falling levels). Below the menu-settings of an alarm-input is shown.

```
Digital alarm input

[0] Exit
[1] Name                >> Digital alarm
[2] Port mode          >> Port 2: Internal pull up
[3] Digital input      >> High active
[4] Trigger delay      >> 00:00:01
[5] Register value     >> 13 Alarms
[6] Alarm              >> Alarm
[7] Counter            >> Counter
[R] Remove
>
```

4.13.1 Trigger delay

The amount of time the data logger waits before changing to the alarm state (when the input condition is true). When the logger measures an alarming input-condition it enters the pre-alarming mode. This mode will change into alarming mode when the trigger delay has finished. If the alarming condition disappears during this time, the logger will NOT enter alarming mode, but will continue in normal mode.

4.13.2 Register value

Holds the amount of alarms that occurred. The user can edit this value.

4.14 Digital inputs - State input / On-time meter

This feature uses the same electrical input as the previous digital sensors, but it handles the signal differently. This driver can be used to log state transitions (on-off and off-on) and to count the on-time (active time) of the input.

```

Digital state input

[0] Exit
[1] Name           >> Digital state
[2] Port mode     >> Port 2; Internal pull up
[3] Digital input >> Low active
[4] Register value >> 0 hour
[5] Register reset >> Not used
[6] Total on-time >> Total on-time
[7] Interval on-time >> Not used
[8] Input state   >> Not used
[R] Remove
    
```

4.14.1 Total On-time

Is a meter counting the total on-time (active time) of the digital input in hours. This counter could be useful in maintenance application (e.g. monitoring pump operating hours). The on-time is recorded at the general log interval.

4.14.2 Register value

The latest know total on-time, you can set to another value if required (e.g. to zero after replacing a pump).

4.14.3 Register reset

The total on-time meter can run for ever or automatically be set to 0 at particular time at a daily bases.

4.14.4 Interval On-time

Like the Total On-time, but counts the On-time over a log interval only. By applying a factor you can record this interval in minutes or seconds if you like.

4.14.5 Input state

Use to record the state of the input at every log interval and at every state transition.

4.15 Network Signal Sensor

This is an internal sensor that measures the quality of the 2G/3G network signal. This is a very important status measurement, because it is directly related to the connectivity of the data logger. We advise to include this sensor in your configuration, and to monitor this parameter regularly.

```
Network signal sensor

[0] Exit
[1] Name >> Network signal
[2] Independent data log >> 0n
[3] Sample log interval >> 06:00:00
[4] Signal bars (0-5) >> Network signal
[5] Signal (dB) >> Not used
[6] Signal (%) >> Not used
[7] Signal indication >> Not used
[8] Bit error ratio >> Not used
[R] Remove
[T] Signal test >> Passed
>
```

4.15.1 Independent data log

The interval on which this sensor is sampled. This sensor is a virtual sensor, in fact the information is obtained from the internal modem. Because the modem draws a lot of energy, it is not a good idea to use these sensors along with the other sensors at the same interval. It is much more economical to use this sensor only at the send interval. Because the modem has to work on that interval anyway, so you can get this info without losing any extra energy. The name “independent data log” is derived from this situation. Set it according to your needs, but preferably use the send interval as setting.



4.15.2 Signal bars

A comprehensive presentation of the quality of the sensor (the network coverage at your installation site) 0 bars = no reception, it will not work. The system will work from 1 bar and above. Try to setup your (external?) antenna for optimum reception. 3, or more is a very good reception.

4.15.3 Signal dB%/indication/bit error rate

A technical presentation of the quality of the signal. These figures are technical and harder to comprehend. (example: a signal of -34 dB is twice as weak as a signal of -31 dB, dB is a logarithmic presentation. Also, the % presentation is NOT linear.) We advise to use the signal bars.

4.16 Aggregation Channels

The logger is equipped with 8 aggregation channels which can be used to record aggregated values (average, minimum, maximum, gust and standard deviation) calculated over a period of your choosing. The number of samples taken into account during the aggregation period is depending on the period duration and the 'Sample interval' as configured for the used input parameter/sensor.

Each channel has an aggregation buffer of 600 values. So, a 10-minute aggregation period (600 seconds) can be sampled with 1Hz, longer aggregation periods e.g. 20 minutes can be sampled with 1Hz but will cause the use of intermediate averages. As 1Hz is the highest possible aggregation sample rate, shorter aggregation periods will contain less samples (e.g. 120 samples for a 2-minute aggregation interval). An aggregation interval can be shorter or longer than a data log interval, so it's possible to record a 10 minute (rolling) average every 2 minutes. Or record the last 2-minute average every 10 minutes.

With a 1Hz sample rate the logger needs to wake-up and take a sample every second, to avoid draining the batteries the used sensors should require a short warm-up (a fraction of the sample interval) consume as little power as possible preferable none (like a reed switch based anemometer), self-powered (like a pyranometer) or negligible (like a 20KOhm wind vane potentiometer). The power draw is about reversed proportional to the sample interval, a twice longer interval will draw about 50% less power.

```

Configuration setup

[0] Exit
[1] General settings      >> YD0Cb721BK
[2] Modem settings
[3] NTP time update      >> Used
[4] Alarm SMS            >> Not used
[5] Option boards        >> Not used
[6] Internal sensors     >> Internal
[7] Analog sensors       >> Potentiometer
[8] Digital sensors      >> Digital pulse
[9] Network signal sensor >> Not used
[A] Serial port          >> Not used
[B] Accessory port       >> Not used
[C] Derived channels    >> Used
[D] DTU connection      >> Not used
[E] Email output         >> Not used
[F] FTP output           >> Not used
[G] TCP output           >> TCP
[-] HTTP output          >> N/A
>
    
```

```

Derived channels

[0] Exit
[1] Aggregations >> Used
[2] Calculations >> Not used
    
```

Per aggregation channel you have to choose which input/sensor values you want to use for aggregation.

For input type you can choose 'Scalar', 'Direction' or 'dB'.

A normal 'Scalar' value like a windspeed can be averaged by accumulation and division. A direction (0..360 deg) like wind direction needs to be dissolved in two x and y components first and their average combined back into a direction again.

```

Aggregation channel 1

[0] Exit
[1] Input parameter      >> Direction (D)
[2] Input type           >> Direction
[3] Aggregation period   >> 00:10:00
[4] Average              >> Average Direction
[5] Minimum              >> Minimum Direction
[6] Maximum              >> Maximum Direction
[7] Gust                 >> Not used
[8] Deviation            >> Deviation
[9] Percentile 1         >> Not used
[A] Percentile 2         >> Not used
[B] Percentile 3         >> Not used
[R] Remove
>
    
```

E.g. a northern wind flapping between 340 and 10 degrees will result in an average northern wind of 355 instead of a faulty 175 degrees southern wind.

Some values (like Noise) are expressed in dB and as dB is a logarithmic value the individual values have to be linearized first before averaging (e.g. the average of 10dB +20dB is not 2 but 17.4dB).

Choose an aggregation period, a commonly used wind speed aggregation period is 10 minutes. Each aggregation buffer can hold max 600 values, so values for a 10 minute aggregation can be sampled with 1Hz. If you want a 20 min aggregation sampled with 1Hz, then 2 second averages will be used.

4.16.1.1 Average, minimum, maximum and standard deviation

Choose which aggregation results you want to record, being average, minimum, maximum, standard deviation and/or gust. A gust is the highest 3 sample average occurred in an aggregation period.

4.16.1.2 Percentiles

It's also possible to define up to 3 different percentiles in ascending or descending order. E.g. to determine the background noise in a certain area you can sample the noise in dBA and take the 95% percentile of all sample noise values in descending order. The value returned (LA95) will be the noise level not exceeded by 95% of the values. The noise peak load (LA10) can be determined by taking the 10% percentile in descending order. A 50% percentile will give the median.

4.17 Calculation Channels

Besides the different Physical channels, the data logger contains, it also has a number of “calculation channels”. These are very powerful, virtual channels. i.e. they are not real physical input channels, but virtual channels to hold i.e. an in between result, for a complex calculation. It allows the user to perform complex calculations in order to transform the electrical signal from the input to a real-life value. It enables the user the connection of a very wide range of sensors, including non-linear ones. All kind of mathematical functions can be used inside a calculated channel. The section covers how to use calculated channels and gives you a real-life example. Calculated channels are found in the configuration setup (below)

```

Configuration setup

[0] Exit
[1] General settings      >> YD0C6721BK
[2] Modem settings
[3] NTP time update     >> Used
[4] Alarm SMS          >> Not used
[5] Option boards      >> Not used
[6] Internal sensors   >> Internal
[7] Analog sensors     >> Potentiometer
[8] Digital sensors    >> Digital pulse
[9] Network signal sensor >> Not used
[A] Serial port        >> Not used
[B] Accessory port     >> Not used
[C] Derived channels    >> Used
[D] DTU connection     >> Not used
[E] Email output       >> Not used
[F] FTP output         >> Not used
[G] TCP output         >> TCP
[-] HTTP output       >> N/A
>
    
```

```

Derived channels

[0] Exit
[1] Aggregations >> Used
[2] Calculations >> Used
>
    
```

A calculated channel can be used to derive a meaningful engineering value from sensed input values using mathematical operators, parentheses and functions (a/o cos, sin, atan2, ln, sqrt).

4.17.1 Syntax

Within the data logger each sensed/calculated parameter/channel has a parameter code chosen by the user (e.g. TEMPC for a temperature in Celsius, **Note:** codes should not contain any spaces or signs). These parameter codes can be used in equations by preceding them with a colon (:). When calculating the parameter codes will be substituted with the last recent measured values. It's possible to use multiple parameters in one equation. The order of operations (add, subtract, divide and multiply) is the same as when using a calculator and parentheses can be used to group operations together if you are confused about the order of operation.

4.17.2 Functions

Besides using simple operators, mathematical functions can be used as well. The syntax of a function is: <function_name>(<arguments>).

Example: sin (x) (calculates the sinus of x)

4.17.3 Example 1


A measured tank liquid level could be compensated with temperature and passed thru an equation to calculate the contents of the tank in kg.

```
Channel 1
[0] Exit
[1] Parameter >> Temp F
[2] Formula >> round( (:TEMPC*1.8+32)*10)/10
[-] Result >> 90.1
[R] Remove
>
```

Within the data logger each sensed parameter/channel has a parameter code chosen by the user (e.g. TEMPC for a temperature in Celsius). These parameter codes can be used in equations by preceding them with a colon (:). When calculating the parameter codes will be substituted with the last recent measured values. You could enter the equation **round((:TEMPC*1.8+32)*10)/10** to convert a temperature in Celsius to Fahrenheit and round the result to one decimal.

4.17.4 Example 2

Assume we measure a river height in m (parameter code LEVEL) and want to convert it to a flow by using the pre-determined polynomial: (see graph below) $y = -0.253x^3 + 21.675x^2 - 359.14x + 1677.5$
Then the formula should be entered as follows: $-0.2535*\text{pow}(:\text{LEVEL};3) + 21.675*\text{pow}(:\text{LEVEL};2) - 359.14*:\text{LEVEL} + 1677.5$

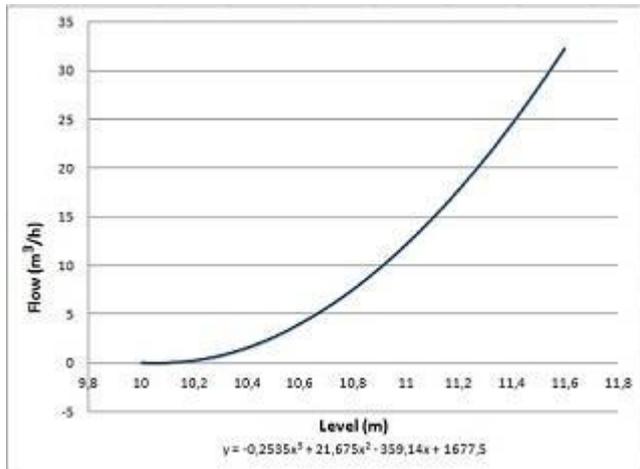

4.17.5 Supported mathematical functions with one argument:

4.17.5.1 abs(x)

returns the absolute value of x

Example: abs(10.7)= 10

4.17.5.2 sqrt(x)

returns the square root of x

4.17.5.3 ln(x)

returns the natural logarithm of x

4.17.5.4 exp(x)

calculates the exponent of e to x

4.17.5.5 log(x)

returns the base 10 logarithm of x

4.17.5.6 sin(radians)

returns the sinus of radians

4.17.5.7 cos(radians)

returns the cosine of radians

4.17.5.8 tan(radians)

returns the tangent of radians

4.17.5.9 asin(x)

returns the arc sinus of x in radians

4.17.5.10 acos(x)

returns the arc cosine of x in radians

4.17.5.11 atan(x)

returns the arc tangent of x in radians

4.17.5.12 torad(degrees)

converts degrees to radians

4.17.5.13 todeg(radians)

converts radians to degrees

4.17.5.14 floor(x)

returns the largest integer not greater than x

4.17.5.15 ceil(x)

returns the smallest integer not less than x

4.17.5.16 round(x)

rounds to the nearest integer

4.17.6 Supported mathematical functions with multiple arguments:

4.17.6.1 atan2(x;y)

return the arc tangent of x/y

4.17.6.2 mod(x;y)

return the remainder of x/y

4.17.6.3 pow(x;y)

returns x to the power of y

4.17.6.4 clip(x;min;max)

returns x clipped between min & max

Example: clip(5;0;100) returns 5

Example: clip(-10;0;100) returns 0

Synonym: If(x<min) return min;Else if(x>max) return max; Else return x

4.17.7 Supported comparisons with 2 arguments:

4.17.7.1 lt(x;y)

returns x if x smaller than y else return y

Example: lt(10;11) returns 10; Synonym: If (x<y) return x; else return y

4.17.7.2 le(x;y)

returns x if x smaller or equal than y else return y

Example: le(10;11) returns 10; Synonym: If (x<=y) return x; else return y

4.17.7.3 gt(x;y)

returns x if x greater than y else return y

Example: gt(10;11) returns 11; Synonym: If (x>y) return x; else return y

4.17.7.4 ge(x;y)

returns x if x greater or equal than y else return y

Example: ge(10;11) returns 11; Synonym: If (x>=y) return x; else return y

4.17.8 Supported comparisons with 4 arguments:

4.17.8.1 eq(x;y;q;p)

returns q if x is equal to y else return p

Example: eq(10;11;0;3) returns 0; Synonym: If (x==y) return y; else return p

4.17.8.2 lt(x;y;q;p)

returns q if x smaller than y else return p

Example: lt(1;2;3;4) returns 3; synonym: if(x<y) return q; else return p

4.17.8.3 le(x;y;q;p)

returns q if x smaller or equal than y else return p

Example: le(1;2;3;4) returns 3; synonym: if(x<=y) return q; else return p

4.17.8.4 gt(x;y;q;p)

returns q if x greater than y else return p

Example: gt(1;2;3;4) returns 4; synonym: if(x>y) return q; else return p

4.17.8.5 ge(x;y;q;p)

returns q if x greater or equal to y else return p

Example: ge(1;2;3;4) returns 4; synonym: if(x>=y) return q; else return p

4.17.9 Various supportive functions:

4.17.9.1 pi

returns 3.1415926

4.17.9.2 time

returns seconds since midnight local time.

Example: 43200 is 12:00:00 and 86399 is 23:59:59

4.18 Serial Port

The serial port of your data logger provides different forms of serial communications. This chapter describes the details of this communication.

4.18.1 RS232

This mode allows to connect to RS232 sensors, see [RS232](#) for details of the electrical properties. Below a menu-settings screen is shown, for an RS232 sensor.

```

RS232 sensors

[0] Exit
[1] Generic MODBUS/RTU
[2] Generic Serial
[3] Generic NMEA
>
    
```

4.18.2 Generic Modbus

This is a versatile protocol that can be used with RS232, but you'll encounter it more frequent with RS485. Modbus is a compact protocol that is the factory standard for RS485 communications. So, when you use RS485, you can also select Modbus, in fact, it's the only option for RS485. Below the settings menu for Modbus is shown:

```

[0] Exit
[1] Name >> MODBUS
[2] Port settings >> RS232 8N1; 19200 Baud; Address 1
[3] Sensor power switch >> Enabled; Warm up 00:00:01
[4] Sample interval >> Data log interval
[5] Protocol type >> RTU
[6] Start command >> Not used
[7] Ready status >> Not used
[8] Ready after/within >> 00:00:01
[5] Register type >> Holding
[6] Register address >> 0
[7] Data type >> WORD (unsigned 2 bytes)
[8] Parameter 1 >> Not used
[9] Parameter 2 >> Not used
[A] Parameter 3 >> Not used
[B] Parameter 4 >> Not used
[C] Parameter 5 >> Not used
[D] Parameter 6 >> Not used
[E] Parameter 7 >> Not used
[M] More parameters >> Not used
[R] Remove
    
```

4.18.2.1 Port Settings

The user can select the right baud rate and Modbus Address of his sensor here. The address of the sensor is very often adjustable, with the aid of a configuration tool of the sensor's manufacturer. So, the user can change this according to its need. You can build a multi-sensor network, by using unique addresses.

4.18.2.2 Protocol type

Choose the MODBUS protocol type: RTU or ASCII

4.18.2.3 Start command

If your sensor does not start measuring automatically after power on, but requires a start command. Please specify which register and value should be written to inform the sensor to start measuring.

4.18.2.4 Ready status

If sensor values are not immediate valid after a power on or after issuing a start command, it would be ideal when a sensor is equipped with a status ready register, if so please specify its register address and the value it contains when sensor values are supposed valid. The logger will not record any sensor value until this register is set to the 'ready value'.

4.18.2.5 Ready after

If no 'Ready status' is defined, the 'Ready after' value indicates the time to wait after sensor warm-up or issuing a start command before sensor values are considered valid.

If a 'Ready status' is defined, the 'Ready within' value is the maximum time(out) the logger will poll for the "Ready status".

4.18.2.6 Register type

Consult the manual of your sensor for this. 3 types are supported:

- Bit register
- Holding register (default register)
- Input register

4.18.2.7 Register Start address

This is the Modbus address of the sensor parameter of your interest. Very often more than just one register contains information, so the data logger starts here, and reads up to the number of bytes needed to fill the selected data type.

4.18.2.8 Data Type

The type of the data that is stored in the sensor @ the starting address. See table below.

Datatype	Size	Signed	Remarks
WORD	2 bytes	unsigned	
Short	2 bytes	signed	
DWORD	4 bytes	unsigned	
Integer	4 bytes	signed	
Float	4 bytes		IEEE754

All 4 bytes data types are also available for reversed logic. (byte swapping)
Consult your manual what data type is used to represent your data value.

The collected data is stored in the selectable parameter(s) The user can modify the collected value if he likes, it is just a generic parameter. More on parameters see [Parameters](#)

4.18.2.9 Timing

The logger expects the sensor to respond within 1 second after issuing a request and will try the request up to 3 times if not.

4.18.3 Generic Serial

This is based upon a serial device that autonomously outputs sentences of data, like an GPS device. The user can capture this data, split it into various parameters, by specifying a separator character and by specifying the start and stop characters of a data sentence. If a serial sensor outputs multiple different sentences, like an NMEA-0183 device, a parameter can be linked to a matching sentence by supplying a sentence filter text.

```

[0] Exit
[1] Name >> Serial
[2] Port settings >> RS232 8N1; 9600 Baud
[3] Sensor power switch >> Enabled; Warm up 00:00:01
[4] Sample interval >> Data log interval
[5] Maximum wait time >> 00:00:10
[6] Log raw data string >> Off
[7] Decimal symbol >> '.'
[8] Separator character >> ','
[9] Start character >> '$'
[A] Start character 2 >> (None)
[B] Stop character >> (CR)
[C] Output request string >>
[D] Output request terminator >> (CR)

[P] Parameters >> 3
[R] Remove
>

```

4.18.3.1 Log raw data String

The user can select this to log the whole data string, including separator char's, checksums etc. This is convenient when debugging / testing a new sensor.

4.18.3.2 Decimal symbol

The user can select which decimal symbol is used by the sensor, being a dot or a comma.

4.18.3.3 Separator Character

Character which separates the various data fields (numbers). Very often a space (0x20) is used. This is the default-setting. A comma, semi-colon or tab-character are commonly in use as well.

4.18.3.4 Start/Stop character

These define with which character a data sentence starts and terminates. E.g. an NMEA sentence starts with a '\$' and terminates with a carriage return (CR).

4.18.3.5 Output request

Most serial probes start transmitting their data sentences at regular intervals as soon as they got powered. Some serial probes output their data sentences on request only and for such cases you can specify an optional "Output request string" and/or "Output request terminator" character. The request string will send first to the probe directly followed by the request terminator (e.g. a carriage return or line feed).

4.18.3.6 Parameters

These are the values you want to get recorded from the data sentence(s).

Each parameter has 3 properties.

```

Serial parameter input settings

[0] Exit
[1] Sentence filter    >> MWV
[2] Field position    >> 1
[3] Field type        >> Numeric
[4] Parameter settings >> Wind direction
>
    
```

4.18.3.7 Sentence filter

If a serial device can output multiple different sentences you can distinguish them from each other by specifying a sentence filter text to capture your parameter from the correct matching sentence. You can leave the filter 'blank', if the device outputs one type of sentence only.

4.18.3.8 Field position

A captured sentence is split up in multiple fields based on the chosen separator character. The first field starts has position number 0.

4.18.3.9 Field type

The format of the field vale, this can be a 'Numeric' ASCII presentation (e.g. -123.45), a 'Hexadecimal' ASCII presentation (e.g. 00FF) or a single character. Note: a single character will be recorded as a its ASCII numeric value (e.g. 'A' will be recorded as 65).

4.18.3.10 Example:

An NMEA-0183 compliant weather station could output the wind direction and speed with the following sentence. This sentence contains 6 comma separated fields.

```
$WIMWV,190.0,R,11.0,N,A*1B
```

```

Serial parameter input settings

[0] Exit
[1] Sentence filter    >> MWV
[2] Field position    >> 1
[3] Field type        >> Numeric
[4] Parameter settings >> Wind direction
>
    
```

The 'Wind direction' value is found at position 1 in the sentence and the sentence can be distinguished from other NMEA sentence by specifying 'MWV' as the 'Sentence filter'.

4.18.4 Generic NMEA

Similar to 'Generic serial'-driver, but you don't have to specify start/stop and separation characters as they are defined by the NMEA-0183 protocol. Additionally, the 'Generic NMEA' driver supports the NMEA-0183 checksum verification.

4.18.4.1 GPS

\$GPGGA,172814.0,3723.46587704,N,12202.26957864,W,2,6,1.2,18.893,M,-25.669,M,2.0,0031*4F

When using the 'Generic NMEA' driver instead of the 'GPS' driver to input GPS coordinates you might need to do a conversion from dddmm.mmmm N/S/E/W format to +/- ddd.dddddd format. This can be accomplished by using a calculated channel for both the latitude and the longitude.

Latitude formula:

$$(\text{floor}(:\text{GGA}2/100) + ((:\text{GGA}2/100) - \text{floor}(:\text{GGA}2/100)) / 60) * \text{eq}(:\text{GGA}3; 83; -1; 1)$$

Longitude formula:

$$(\text{floor}(:\text{GGA}4/100) + ((:\text{GGA}4/100) - \text{floor}(:\text{GGA}4/100)) / 60) * \text{eq}(:\text{GGA}5; 87; -1; 1)$$

Assuming: GGA2 is the latitude (2nd field position), GGA3 is the direction (3th field, 83='S')
GGA4 is the longitude (4th field position), GGA5 is the direction (5th field, 87='E')

4.18.5 RS485

This is solely used for Modbus communications. For info see: [Generic Modbus/RTU](#)

4.18.6 SDI-12

Used for SDI-12 communications, see below. For generic information on SDI-12 see: [SDI-12](#)

```
SDI12 sensor

[0] Exit
[1] Name >> SDI12
[2] Port settings >> SDI12; 1200 Baud; Address 0
[3] Sensor power switch >> Enabled; Warm up 00:00:01
[4] Sample interval >> Data log interval
[5] Measurement command >> 0C!
[6] Parameter 1 >> Par1
[7] Parameter 2 >> Not used
[8] Parameter 3 >> Not used
[9] Parameter 4 >> Not used
[A] Parameter 5 >> Not used
[B] Parameter 6 >> Not used
[C] Parameter 7 >> Not used
[D] Parameter 8 >> Not used
[E] Parameter 9 >> Not used
[M] More parameters >> Not used
[R] Remove
>
```

4.18.6.1 Measurement command

The user can choose between concurrent measurements (c), or non-concurrent (m). When the sensor supports concurrent measurements, we strongly advise to use it. Because it saves a lot of energy. (all sensors are measuring simultaneously). The command number is asked by the firmware, for retrieving the right data value. For more info consult your sensors manual. After selecting the right measurement command, the command is displayed in the menu, so the user can check this against the sensors manual

4.18.6.2 Parameters

The various data values that were retrieved from the SDI-12 sensor, can be stored into different parameters. They behave like normal generic parameters. See more info: [Parameters](#)

4.18.7 Accessory port

This is a serial port which is used for supporting special serial devices, called accessory port modules. The accessory port is only equipped on the MLx15-ADS models, and the ML2013 data logger. Below a list of supported accessories is shown.

```

Accessory port modules

[0] Exit
[1] Display
[2] Camera
[3] GPS
[4] Radio
[5] Iridium Satellite
[6] Gonets Satellite
>
    
```

These are the accessory modules that can be connected to the accessory-port. Each option is described below. For detailed information consult the manual of the accessory.

4.18.8 Radio

This option is used to send the measured data via a radio module to another system. The radio must be a transparent connection. The brand is not important. Name, port settings, Module power switch is the same as used with input ports, so, not explained here. Also this driver can be used to send serial data to a custom system, via wire.

```

Radio settings

[0] Exit
[1] Name >> Radio
[2] Port settings >> RS232 8N1; 4800 Baud
[3] Module power switch >> Enabled; Warm up 00:00:01
[4] Send interval >> 00:00:10
[5] Send delay >> Not used
[6] Power down delay >> 00:00:05
[R] Remove
>
    
```

4.18.8.1 Send interval

The send interval on which the data is send to the radio. This can be another send interval than the internal modem has. More on send interval see: [Send Interval](#)

4.18.8.2 Send delay

When the user likes an time offset in respect to the send interval he can set this offset here. This is practical, using multiple radio's they must NOT be sending simultaneously. The send interval can be the same for each data logger, but each data logger must have a different send delay, in order to avoid the radios to transmit simultaneously.

4.18.8.3 Power down delay

The logger is often faster than the connected radio device. When the logger has send its data string to the radio, the radio needs some time to send it over the air. This time is defined here (default 5 seconds).

4.18.9 Iridium Satellite

This option is for using satellite communication for data transfer. Not all satellite modems can be used on the data logger. It is designed to work with modems based on Iridium SBD 960x transceivers. We recommend the: <http://www.your-data-our-care.com/datalogger-EDGE-satellite-transceiver.html> as it supports RS-232 and has a weatherproof enclosure with integrated antenna.

The satellite transceiver can be deployed as the data logger's main communication device or as backup in case the 2G/3G network is temporarily unavailable or out of reach. This backup function could be very interesting for traveling data logging applications or remote location at the edge of 2G/3G coverage.

Satellite communication requires the transceiver to have a **clear view at the sky** e.g. it won't work well inside buildings or under the canopy of trees. By using "comport redirect" (see: Maintenance Menu - Field testing) you can check the signal strength by issuing the AT+CSQ command or even try to send a text message with the AT+SBDWT command. Please download http://www.your-data-our-care.com/download/ISU_AT_Command_Ref.pdf for a full description of these and other AT commands.

4.18.9.1 Iridium SBD Service



Download : http://www.your-data-our-care.com/download/IRDM_IridiumSBDService.pdf for more info.

SBD messages are transmitted to an Iridium server (GSS: Gateway Short Burst Data Subsystem) and you can ask your Iridium provider to pass SBD messages to an e-mail address of your choosing or via IPdirect to an IP-address/domain and TCP-port of your choosing. When using your own software, you have to either pick-up and import the e-mails or implement a TCP-server to receive SBD messages.

We have implemented two flavors of SBD messages: "Text" and "Compacted".

The body of an "Text" message contains one timestamped log record at max.
The body of an "Text" message is formatted as follows:

```
*<logger s/n>;<yyddmmhhmmss>;<par code1>;<par value1>;...;<par codex>;<par valuex>
```

Example: *5304783;160513140000;TEMP;23.6;LEVEL;3.32;BATT;4.2

See chapter: "Compacted Data Format" for a description of the "Compacted" SBD message format.

When using ydoInsights you should ask your Iridium provider to use IPDirect and pass SBD messages to the same IP-address/domain and TCP-port as used for 2G/3G TCP-output from common YDOC data loggers.

4.18.9.2 Settings menu

```

Iridium Satellite settings

[0] Exit
[1] Name                >> Iridium Satellite
[2] Port settings      >> RS232 8N1; 19200 Baud
[3] Module power switch >> Enabled; Warm up 00:00:20
[4] Send interval      >> 01:00:00
[5] Send delay         >> Not used
[6] Data transpond     >> Actual values
[7] Backup mode        >> Not used
[8] Message format     >> Compacted
[R] Remove
  
```

4.18.9.3 Send interval

The send interval on which the data is send by satellite communication. Beware that satellite communication is rather expensive, so please choose a moderate Send interval and consider the use of the aggregation features of the data logger (e.g. sample evert 5 minutes, but only record an hourly average). In case satellite communication is used as backup, the send interval is determined by the primary communication channel, but only when primary communication fails.

4.18.9.4 Data transpond

As satellite communication is rather expensive you can choose to send only the last sampled values instead of logged values. When choosing to transpond logged values be aware to select a moderate log interval to avoid high communication costs.

Note: only parameters with the 'Data transpond' flag enabled will be included in an SBD message.

4.18.9.5 Backup mode

When the 'Backup' mode is selected satellite communication will be performed only if data transfer by TCP, FTP, e-Mail or HTTP thru the cellular network is failing. You can also specify the number of cellular transmission failures before satellite transfer takes place. When you set failures to 3 data transfer by satellite will be performed every third cellular data transmission failure.

4.18.9.6 Message format

The SBD messages can be transmitted in readable ASCII or in a compacted binary format. The compacted binary format is about 20 to 80% more efficient saving a lot of communication costs, but needs specific processing to be able to interpret the message (The ydoInsights data collector is provisioned with the algorithms to interpret the message).

See chapter "Compacted Data Format" for a description of this format.

The compacted format is limited to contain up to 15 logger parameters/channels. As textual parameter codes would use too much data, the identification of the individual channels is based on a number between 1 and 15. Assigning the numbers to individual parameters is a matter of configuration by starting their code names with a capital P followed by a number between 1 and 15. The P will be stripped of, as well as any trailing characters, so you could specify meaning full codes like: P1TMP or P02HUM or P15LEV. Make sure that the number parts are unique and the "Data transpond" option of the concerned parameters is enabled as well.

4.18.10 GPS

This is the driver for a standard NMEA-GPS. Some settings are discussed below. Although every standard NMEA-GPS can be used, it is convenient to use an YDOC-GPS, because it can be powered from the accessory port also. YDOC GPS is found on: http://www.your-data-our-care.com/data_logger-GPS-E3329-receiver.html

Note: If GPS sentences are combined with other NMEA sentences with measurement data you want to log, its recommended to use the 'Generic NMEA' driver instead of this 'GPS' driver.

```

GPS settings

[0] Exit
[1] Name >> GPS
[2] Port settings >> RS232 8N1; 9600 Baud
[3] Module power switch >> Enabled; Warm up 00:00:10
[4] Independent data log >> 0n
[5] Sample log interval >> 06:00:00
[6] Minimum satellites to use >> 3
[7] Minimum wait time to Fix >> 00:00:00
[8] Maximum wait time to Fix >> 00:01:00
[9] Log raw data string >> 0ff
[A] Calculate alarm limits on deployment >> 0ff
[B] Latitude hi/lo alarm drift >> 1 sec
[C] Longitude hi/lo alarm drift >> 1 sec
[D] Latitude hi-hi/lo-lo alarm drift >> 3600 sec
[E] Longitude hi-hi/lo-lo alarm drift >> 3600 sec
[F] Satellites >> Satellites
[G] Latitude >> Latitude
[H] Longitude >> Longitude
[I] GPS quality >> Not used
[R] Remove
>

```

4.18.10.1 Minimum satellites to use

The GPS can calculate a position based upon the data of multiple satellites, the minimum amount of satellites for this calculation is 3. But the calculation gets better, when more satellites are used. This parameter defines the minimum number of satellites that is used during the calculation. The data logger tracks the SVS (space vehicles) parameter from the GPS output string to determine this. So, the data logger will wait for the SVS in the data string to be equal or more than this figure.

4.18.10.2 Time to fix

A GPS receiver has a certain time to Fix (TTF). This is the time from power-on to the calculation of a valid position. The data logger knows 2 limits to define the timeframe in which it waits for a fix. These are minimum wait time to fix and maximum wait time to fix. Please use these according the specs of your GPS. Of course, when a position is found, within the range of this timeframe, the position will be stored, and the logger will proceed to his next task. If the fix is NOT found, a sensor timeout will occur.

4.18.10.3 Position drift alarming

This is a feature that simplifies the process of setting up an alarm on the position of the device. Sometimes, it is important to track the position of the system, and to couple an alarm to it. I.e. with buoys this might be the case. The buoy must measure on a specific location and may drift a few meters, but must not drift too far. To setup an alarm, with the corresponding limits is very unpractical, because the user has to work with the coordinates, coming from the GPS, and they are not comprehensive at all. Also, very often, the user has a good idea about the maximum allowable drift of the buoy, but NOT yet the starting location of it.

4.18.10.3.1 Calculate alarm limits on deployment

This feature helps the user to set up a region which will be guarded by the data logger. This region can be setup at the office, far away from the installation site. The region is setup by defining the size of a rectangular, in which the buoy is supposed to operate. The buoy can drift in this box, without causing an alarm. The parameters of this box are:

4.18.10.3.2 Latitude/Longitude hi/lo alarm drift

Both limits represent (geographical) seconds, and likewise, a box is created with the size of 2 times the latitude hi/lo alarm drift by 2 times longitude hi/lo alarm drift. So, this box has a user defined size, but is unrelated to the position of deployment. At deployment, these values are automatically related to the (starting) position of the system. It automatically calculates the alarm limits for the parameters latitude and longitude. Thanks to this, the user can define a "box of allowed movement" at the office, and during deployment, the absolute alarm limits for latitude and longitude are calculated.

Also, the user can define a second, bigger, box, which corresponds with the hi/hi limits of the data logger. So, a second level of alarming can be defined.

4.18.10.4 Satellites

The amount of satellites, used in the calculation of the position. This parameter is retrieved from the standard NMEA string.

4.18.10.5 Latitude / Longitude

Notation of the position, in the WSG84 system,

4.18.10.6 GPS Quality

Quality of the measurement. More info on this is found in the manual of your GPS.

4.18.11 Camera

This is used to connect an YDOO camera only. It shoots a picture and stores it on the SD-card for transmission to the host. More info on this camera's is found here: <http://www.your-data-our-care.com/data-logger-accessories.html>

Below the settings are shown

```

Camera settings

[0] Exit
[1] Name >> Camera
[-] Port settings >> RS232 8N1; 115200 Baud
[3] Accessory power switch >> Enabled; Warm up 00:00:05
[4] Independent data log >> 0n
[5] Sample log interval >> 06:00:00
[6] Interval shift >> Not used
[7] Instantaneous picture >> 0ff
[8] Picture size >> 640x360(16:9), 640x480(4:3)
[9] Picture sending >> None
[A] Picture storage >> Delete after send
[B] Picture number >> Picture
[R] Remove
[T] Camera test >> Not done
>>
    
```



Select you proper picture size, according your needs, and your camera. Please consider that a high-resolution picture results in more data and also more power required. So don't exaggerate with the picture-size. The pictures can be send to you by: HTTP, E-mail, FTP, TCP or MQTT.

For an estimation of power consumption and payload, please visit: <http://www.your-data-our-care.com/data-logger-power-consumption.html>

Pictures can be taken independent from the normal data logging interval, e.g. once a day (Interval: 24:00:00) at 9h (Shift with 09:00:00). You can also use a switch to ground on 'Digital input 1' to take an instantaneous picture.

For more information on the camera, please visit: <http://www.your-data-our-care.com/data-logger-accessories.html>

4.18.12 Display

This driver is intended for the operation of an YDOC display unit. With this display unit, the measurements can be consulted, locally, in a graphical way. The YDOC display unit is a 3.5" colour resistive touch screen display with a resolution of 320*240 pixels.



Display settings

```

[0] Exit
[1] Name          >> Display
[-] Port settings >> RS232 8N1; 115200 Baud
[3] Power down delay >> 00:01:00
[R] Remove
>
    
```

4.18.12.1 Power down delay

This is the time, the data logger shuts the display down, after not touched anymore. With this accessory you can recall graphs, or numeric, actual values of all parameters. It has an auto-scale feature for graphing and allows the user to browse the history of the measurements (via the graphs).

4.18.12.2 Order of parameters

The display can show up to 6 parameters simultaneously organized in two columns and three rows. 'Next'- and 'Previous'-buttons can be used to shift columns in & out of view when having more than 6 parameters. The columns are ordered from left to right and their row items from top to bottom.

See chapter "Parameter overview" to alter the order of parameters.



4.19 Email output

This output driver is used to send the collected data from the SD Card to a mailbox of the user. The data is included in an attachment of the email. Below the settings are shown: Some of its settings are commented below, other settings are generic and covered before in this manual.

```

Email settings

[0] Exit
[1] Name                >> Email
[2] Send interval      >> 01:00:00
[3] Send delay         >> Not used
[4] SMTP server        >>
[5] SMTP port          >> 587
[6] Security           >> Basic
[7] Username           >>
[8] Password           >>
[9] Originator address >>
[A] Destination address >>
[B] Subject            >>
[C] Output type        >> Log data
[D] Data format        >> Native(txt)
[E] Data format        >> Data & Diagnostics
[R] Remove
[T] Email test         >> Not done
>

```

4.19.1 Server

This is the IP-address or domain name of the SMTP-server you want to use for e-mailing. You can use you ISP's server, or any other server you like.

4.19.2 SMTP port

Port on which the SMTP server is listening. There is something interesting to say about this: SMTP uses the well-known port 25. In the early days, this port was always used. But nowadays, the providers are using different port numbers. They have their own SMTP-server, which work on international standard port 25, and they don't allow traffic on this port except for their own server. Therefore, a problem arises. So, in order to solve that, many providers open a second port for SMTP. And our data logger is supporting that. So you can use this anytime.

4.19.3 Security

The data logger supports basic SMTP (credentials and data unencrypted) or encrypted SMTP over TLS.

4.19.4 Originator address

This is the email address of your system. Please note that some ISP's block strange addresses, so make sure to use a serious address, or make sure that it is not blocked by the ISP.

4.19.5 Destination address

This is the email address to where the data is send.

4.19.6 Remote configuration

Not supported, if you want remote configuration possibilities use MQTT, FTP, HTTP or TCP output instead.

4.20 FTP Output

This is for sending data to an FTP- or FTPS-server, see details below

```

FTP settings

[0] Exit
[1] Name >> FTP
[2] Send interval >> 01:00:00
[3] Send delay >> Not used
[4] Server >> your-data-our-care.com
[5] Port >> 21
[6] FTP mode >> Active
[7] Security >> TLS(explicit)
[8] Username >> YDOC
[9] Password >> ****
[A] Directory >> logfiles
[B] Output type >> Log data
[C] File name >> YDOC_SITE-01_99021374_190328_105809.txt
[D] Data format >> Native(txt)
[E] Data filter >> Data & Diagnostics
[R] Remove
[T] FTP test >> Not done
>
    
```

4.20.1 Server

This is the IP-address or domain name of the FTP-server you want to transfer files to.

4.20.2 Port

Port on which the FTP server is listening, which is 21 by default.

4.20.3 FTP mode

This is to choose between Active or passive FTP. More on this topic see: https://en.wikipedia.org/wiki/File_Transfer_Protocol

4.20.4 Security

The data logger supports basic FTP (credentials and data unencrypted) or secure FTPS (using explicit TLS to encrypt credentials and data).

4.20.5 Directory

The relative path to the destination on your server.

4.20.6 File name

The default file name is formatted as “YDOC_<sysname>_<sn>_<yy><mm><dd>_<hh><nn><ss>” and appended with the file extension (.txt. .csv. or .json).

You can customize the file name to your liking and use substitutions like <sysname> for your “system name”, <sn> for the serial number, <name> for the FTP “driver name” as well as various timestamp tokens like <hh> for a 2-digit hour of the day or <h> for hour of the day without leading 0’s. For a 4 digit year presentation use <yyyy>. **Note that** <m> or <mm> is used for months and <n> or <nn> for minutes.


When all possible substitution tokens (9) are used you will have just 7 characters left to customize the file name, but you could manipulate the file by specifying the “system/driver” names wisely. i.e use the “system name” for unique system identification and the “driver name” as a common file name part.

4.20.7 Remote configuration

If the logger has FW V3.0B1 or newer, remote configuration with the data logger can be scheduled by ydocTerminal V3.0. using our secure tunnel server (tunnel.ydoc.biz).

Note: The data logger should be configured to use NTP time synchronization.

Within ydocTerminal click: File->New->Schedule a remote connection.

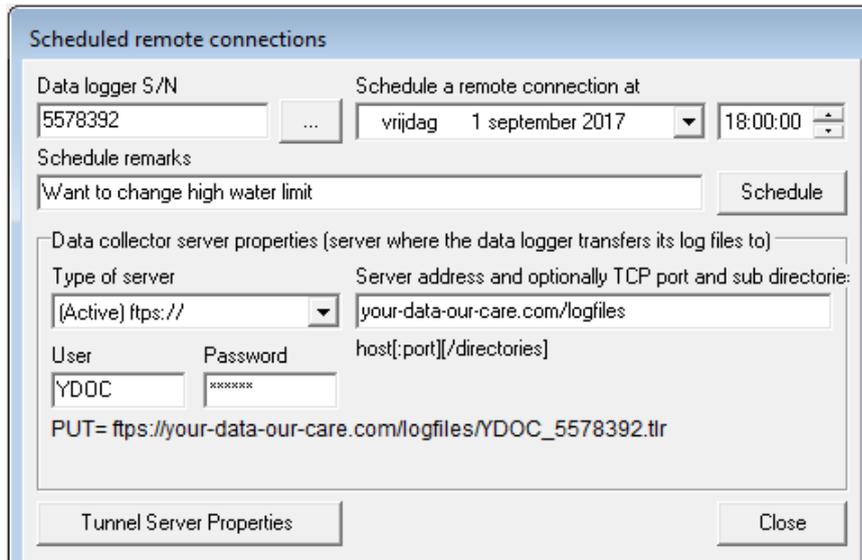

Specify the S/N of the data logger you want to configure and when you think it's a convenient moment to configure the logger.

Obviously: A tunnel cannot be established before the next scheduled data transfer interval of the data logger.

A tunnel can only be established if ydocTerminal is running at the scheduled moment. When running, ydocTerminal will pop-up a terminal window a few minutes before the scheduled moment.

Type of Server

ydocTerminal supports 4 different types of FTP-server (Passive FTP, Active FTP, Passive FTP with Explicit TLS or Active FTP with Explicit TLS).

Server address: Specify the same server and directory as used by the data logger (e.g. your-data-our-care.com/logfiles)

User/Password: Specify the exact same credentials as used by the data logger as they are a/o used in the encryption keys. The user should have read, write and delete rights in the specified directory.

Tunnel Server Properties

This is the Server servicing the secure and encrypted channel between data logger and ydocTerminal. Standard our server is used (tunnel.ydoc.biz), don't worry we can't eavesdrop your data as the communication is 'Peer-to-Peer' encrypted by security keys not know to the tunnel server. If having doubts, please feel free to run your own tunnel server, please ask our staff how to do it.

4.21 HTTP Output

This is for posting data to an HTTP- or HTTPS-server, see details below. The HTTP output is of interest when you are hosting your own monitoring web or cloud server. When using ydocInsights we recommend using TCP output, as TCP-output has far less overhead with less data payload (costs) and less transfer time (power consumption).

```

HTTP settings

[0] Exit
[1] Name >> HTTP
[2] Send interval >> 01:00:00
[3] Send delay >> Not used
[4] Server >> your-data-our-server.com/datacollector/
[5] Port >> 80
[6] Security >> Basic
[7] Username >> YDOC
[8] Password >> *****
[9] Output type >> Log data
[A] Data format >> JSON
[B] Data filter >> Data & Diagnostics
[R] Remove
[T] HTTP test >> Passed
>
    
```

4.21.1 Server

This is the URI of a location on an HTTP-server where log file and camera pictures should be posted to.

When at server-side multiple loggers should share the same URI, the loggers can be distinguished from each other by examining the custom HTTP-header 'X-DeviceSN' which will contain a logger's unique serial number.

4.21.2 TCP port

Port on which the HTTP-server is listening, which is 80 by default for HTTP or 443 for HTTPS.

4.21.3 Security

The data logger supports basic HTTP (credentials and data unencrypted) or HTTPS (using SSL/TLS to encrypt credentials and data).

4.21.4 Data format

This defines the data format of the file to post. This can be our native TXT format, CSV (comma separated value) format or our JSON format which can easily be picked up by server-side scripting of an HTTP-server.

Depending on the data format the following 'Content-Type' HTTP header will be added to the post.

text/plain	Our native TXT format	application/json	Our JSON format
text/csv	CSV format	image/jpeg	A camera picture


If used, camera pictures are posted to the same URI as the log file so you have to examine the 'Content-Type' header to distinguish a picture post from a log file post.

4.21.5 Remote configuration

If the logger has FW V3.0B1 or newer, remote configuration with the data logger can be scheduled by ydocTerminal V3.0. using our secure tunnel server (tunnel.ydoc.biz).

Note: The data logger should be configured to use NTP time synchronization.

Within ydocTerminal click: File->New->Schedule a remote connection.

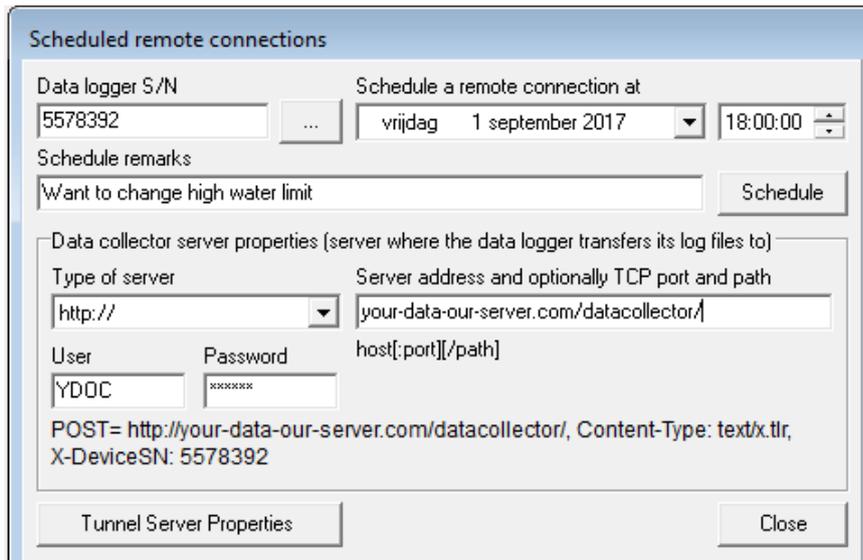

Specify the S/N of the data logger you want to configure and when you think it's a convenient moment to configure the logger.

Obviously: A tunnel cannot be established before the next scheduled data transfer interval of the data logger.

A tunnel can only be established if ydocTerminal is running at the scheduled moment. When running, ydocTerminal will pop-up a terminal window a few minutes before the scheduled moment.

Type of Server: HTTP or HTTPS

Server address: The HTTP-server must honor POST requests from ydocTerminal at the specified URL.

ydocTerminal will POST the request with 'content-type: **text/x.tlr**'. The S/N of the concerned data logger is given in the custom HTTP-header 'X-DeviceSN'. The tunnel link request string itself is contained in the body of the POST. This request string should be stored until the concerned data logger performs a POST itself (its log data). The HTTP-server should copy the request string as the value of the custom HTTP-header 'X-Command' in the response to the data logger.

User/Password: Specify the exact same credentials as used by the data logger as they are a/o used in the encryption keys.

Tunnel Server Properties

This is the Server servicing the secure and encrypted channel between data logger and ydocTerminal. Standard our server is used (tunnel.ydoc.biz), don't worry we can't eavesdrop your data as the communication is 'Peer-to-Peer' encrypted by security keys not know to the tunnel server. If having doubts, please feel free to run your own tunnel server, please ask our staff how to do it.

4.22 MQTT Output

This is for posting data to an MQTT-broker, see details below. The MQTT output is of interest when you want to use a third party IoT monitoring system or smart phone apps supporting generic MQTT. When using ydoc-Insights we recommend using TCP output, as TCP-output has far less overhead with less data payload (costs) and less transfer time (power consumption).

This MQTT driver can be used for sending alarm messages, remote configuration update and firmware upgrade as well, but if you don't want to use the driver to transmit the "Log data", its recommended to schedule the driver to transmit just the "Actual Values" once a day to avoid unnecessary communication payload and according power consumption.

```

MQTT settings

[0] Exit
[1] Name >> MQTT
[2] Send interval >> 01:00:00
[3] Send delay >> Not used
[4] Server >> m21.cloudmqtt.com
[5] Port >> 12656
[6] Security >> Basic
[7] Username >> YDOC
[8] Password >> *****
[9] Root topic >> YDOC/5025064
[A] Client ID >> 359180082361087
[B] Clean session >> No
[C] Data output >> Log data & Actual values
[D] Max payload >> 1000 kB
[E] Data format >> JSON
[F] Data filter >> Data & Diagnostics
[R] Remove
[T] MQTT test >> Passed
>
    
```

4.22.1 Server

This is the IP-address or domain name of the broker to publish to. Most brokers offer free accounts with a connection or payload limit. For mass transfer you might need to use a payed account or run your own MQTT-broker.

4.22.2 Port

The TCP port on which the MQTT-broker is listening, which is 1883 by default or 8883 for MQTT over TLS.

4.22.3 Security

The data logger supports basic MQTT (credentials and data unencrypted) or MQTT over TLS.

4.22.4 Root topic

The MQTT protocol works with so called "Topics" and MQTT clients can subscribe to the "Topics" of their interest (of course in the domain they have access to, you don't want unauthorized entities to subscribe to publications from your equipment).

Within the data logger you can define a "Root topic", which is used as prefix for all "Sub topics". The default "Root topic" is "YDOC/<device serial number>", but it can be changed according to your wishes. E.g. you could define a "Root topic" starting with your own company identification code, followed by some device classification code and your own chosen station identification code.

In example: (ACME/METEOSTATIONS/STATION_001). Your central monitoring system could subscribe to all topics starting with ACME and when a logger publishes for the first time, then your system could create a profile for "STATION_001" based on the specified "METEOSTATIONS" classification.

Clearing the 'Root topic' will set it back to the default YDOC/<SN>

The logger uses the following publishing topics:

- `<root>/sensors/<parameter code>` to publish an "Actual value" of a specific parameter.
- `<root>/data/jsn` to publish the "Log data" in JSON format.
- `<root>/data/csv` to publish the "Log data" in CSV file format.
- `<root>/data/txt` to publish the "Log data" in YDOC native text format.
- `<root>/alarm/sys` to publish "System alarms" in plain text, e.g. about a failing sensor.
- `<root>/alarm/data` to publish "Data alarms" in plain text, e.g. about reaching a low tank level.
- `<root>/jpg/<yymmdd_hhmmss>` to publish "Camera pictures with timestamp" in JPEG format.
- `<root>/status/time` the time of the logger at start of the MQTT session (yyyy/mm/dd hh:mm:ss).

4.22.5 Client ID

Every MQTT client should connect with a unique client identification for which we use the unique IMEI-number of the built in modem. If necessary you can specify your own client ID.

4.22.6 Clean Session


Only check this option if your MQTT-broker requires it, else you won't be able to do remote configuration or "over the air" configuration updates or firmware upgrades anymore.

4.22.7 Max Payload

In circumstances like a network outage a data log file can grow bigger than the maximum topic payload allowed by your MQTT-broker. Please specify the limit if any and the logger will chop the payload in parts.

4.22.8 Remote configuration transfer and firmware upgrade

MQTT can also be used for remote configuration transfer and firmware upgrades thru ydocTerminal.

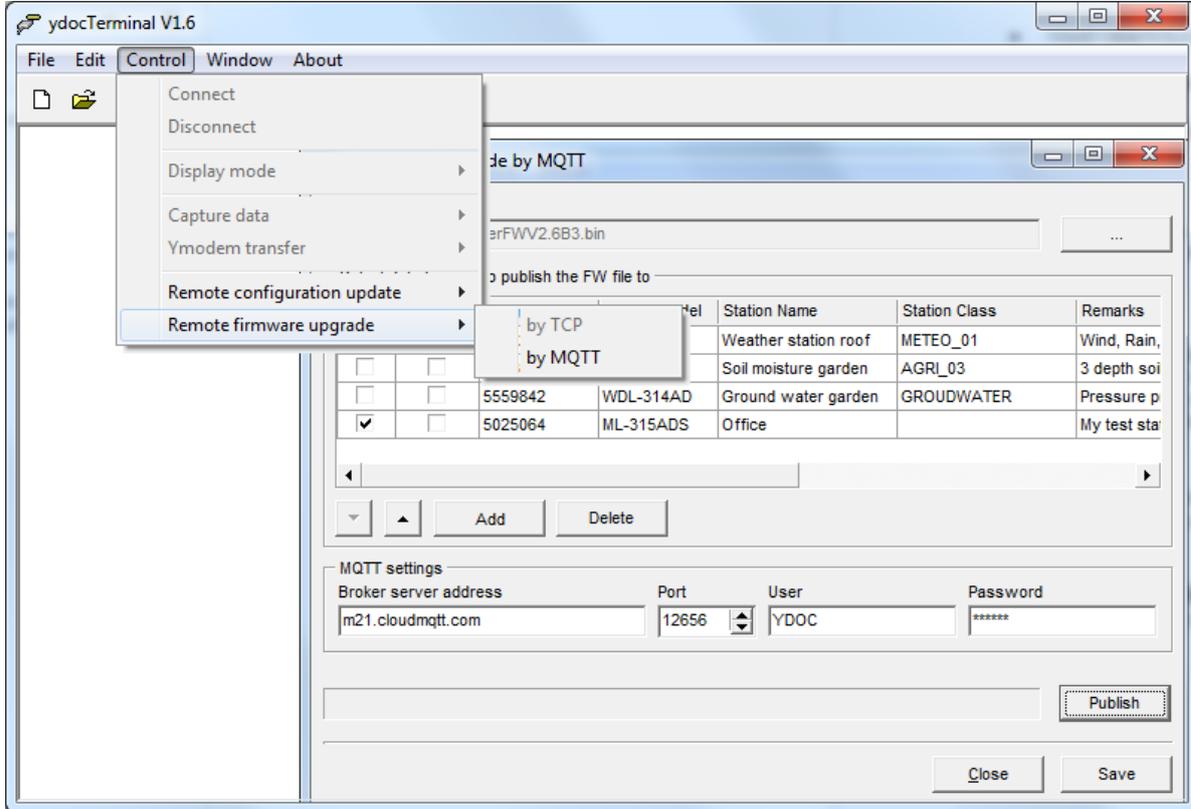


4.22.9 Remote configuration

If the logger has FW V3.0B1 or newer, remote configuration with the data logger can be scheduled by ydocTerminal V3.0. using our secure tunnel server (tunnel.ydoc.biz).

Note: The data logger should be configured to use NTP time synchronization.

Within ydocTerminal click: File->New->Schedule a remote connection.

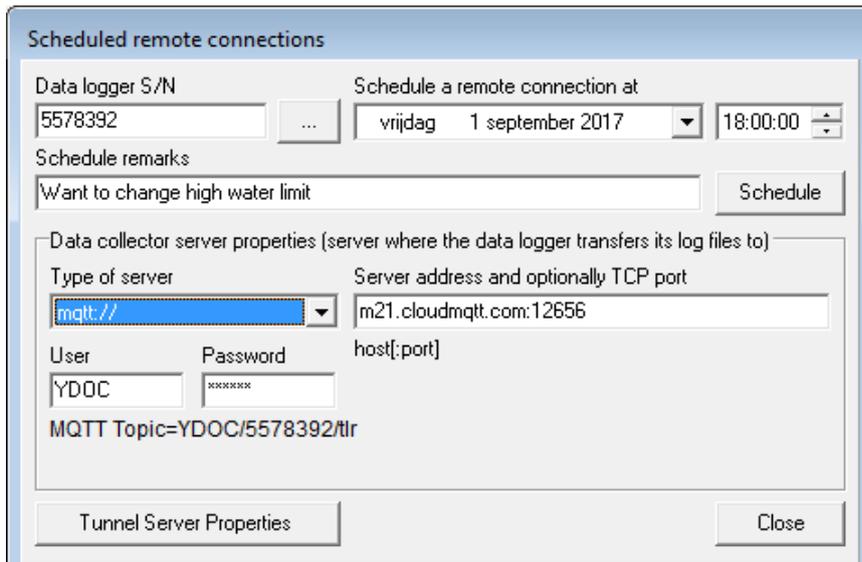

Specify the S/N of the data logger you want to configure and when you think it's a convenient moment to configure the logger.

Obviously: A tunnel cannot be established before the next scheduled data transfer interval of the data logger.

A tunnel can only be established if ydocTerminal is running at the scheduled moment. When running, ydocTerminal will pop-up a terminal window a few minutes before the scheduled moment.

Type of Server: MQTT

Server address: Specify the same server and port as used by the data logger (e.g. m21.cloudmqtt.com:12656)

User/Password: Specify the exact same credentials as used by the data logger as they are a/o used in the encryption keys.

Tunnel Server Properties

This is the Server servicing the secure and encrypted channel between data logger and ydocTerminal. Standard our server is used (tunnel.ydoc.biz), don't worry we can't eavesdrop your data as the communication is 'Peer-to-Peer' encrypted by security keys not know to the tunnel server. If having doubts, please feel free to run your own tunnel server, please ask our staff how to do it.

4.23 TCP Output

This is for sending data to an TCP server, see details below

```

TCP settings

[0] Exit
[1] Name >> TCP
[2] Send interval >> 01:00:00
[3] Send delay >> Not used
[4] Server >>
[5] Port >> 37
[8] Security >> Basic
[6] Username >>
[7] Password >>
[8] Output type >> Log data
[9] Data format >> Native(txt)
[A] Data filter >> Data & Diagnostics
[R] Remove
[T] TCP test >> Not done
>

```

4.23.1 Server

This is the IP-address or domain name of the TCP-server you want to send data to.

4.23.2 Port

Port on which the TCP-server is listening, which is 37 by default. When running your own TCP-server for data collection (e.g. the one that comes with ydoc-Insights) make sure that the chosen port is forwarded by your internet router to the local IP-address of the system/computer running your TCP-server.

See the tutorials at: www.your-data-our-care.com/data-logger-manuals.html

4.23.3 Security

The method used to logon to the TCP-server, this can be 'Basic', 'Secure Authentication' or 'AES-128 encrypted'. When using 'Basic' the credentials are transferred by TCP in plain text. This is quick and therefore consuming less power. When using 'Secure Authentication' the password is uni-directional encrypted with a unique challenge token received from the server. 'Secure Authentication' is more secure but will consume about 1 second more precious power time per transfer. 'AES-128 encryption' includes 'Secure Authentication' and encrypts all communication, this is the most secure and recommend method.

4.24 SMS output

This output driver is used to send the collected data from the SD Card to a cell phone number by SMS. As an SMS is limited in size transferring data by SMS has some limitations too. We recommend to use this driver only if other alternatives are not feasible. Below the settings are shown: Some of its settings are commented below, other settings are generic and covered before in this manual.

```

SMS data settings

[0] Exit
[1] Name          >> SMS
[2] Send interval >> 00:01:00
[3] Send delay   >> Not used
[4] Phone number >>
[5] Data send    >> Log data
[R] Remove
[T] SMS data test >> Not done
>
    
```

4.24.1 Phone number

The cell phone number you want to send data messages to.

4.24.2 Data send

An SMS message is limited to 160 characters, so it's not feasible (like with FTP for example) to send a complete log file in one SMS message. You can choose to configure this driver to only send the last logged record (Actual Values) or all logged records since the last successful data transmission (Log data). Each log record will be sent as an individual SMS message. **Note:** Independ data logs (not part of the regular data log intervals) are not include in SMS data output.

4.24.3 Data format

Each data SMS start with an asterisk, followed by a logger serial number, timestamp and followed by one or more parameter code/value pairs in the same format as with D-record (see: Chapter D-records).

```
*<logger s/n>;<yyddmmhhmmss>;<par code1>;<par value1>;...;<par codex>;<par valuex>
```

Example: *5304783;160513140000;TEMP;23.6;LEVEL;3.32*A;BATT;4.2

4.24.4 Remote configuration

Not supported, if you want remote configuration possibilities use MQTT, FTP, HTTP or TCP output instead.

4.25 Satellite Output (SBD)

A satellite transceiver can be deployed as the data logger's main communication device or as backup in case the 2G/3G network is temporarily unavailable or out of reach. Please read more at chapter "Accessory port – Iridium Satellite".

4.26 Parameter overview

The parameter overview is used to generate an overview of the configuration. It enables the user to evaluate the settings of the logger in an easy way as well as order the order of parameters, it consists of multiple lists:

- Parameter list
- Measurement list
- Alarm list
- Alarm limits

4.26.1 Parameter list

This gives an overview of the configured parameters and their units in a comprehensive ordered list. See example below:

```

Parameter list

Order   Code   Name                               Unit   Dec   Min / Max

[1] 1   AVGci  Average current                   mA     0
[2] 2   OCi    Operating cycle                   sec    2
[3] 3   AVGVl  Average voltage                   V      2
[4] 4   RPi    Rest power                        mAh    0
[5] 5   PTi    Processor temperature            C      1

[0] Exit
>
    
```

You can change the order of a parameter in the list by specifying a new position. To change the position, please click the character between brackets in front of the concerned parameter, this will pop-up a prompt to alter its current position.

4.26.2 Measurement list

This gives an overview of used measurements and its sample rates etc. See example below:

```

Measurement list

Code      Sample interval Alarm interval  Data log   Data transpond

PM        00:00:01      Not used      Off        Disabled
RPT       00:00:01      Not used      On         Disabled
TPT       00:00:01      Not used      On         Disabled
AIN       00:00:10      Not used      On         Disabled
MINVl     00:00:10      Not used      On         Disabled
OCi       00:00:10      Not used      On         Disabled
PTi       00:00:10      Not used      On         Disabled
CNT       00:00:10      Not used      On         Disabled

[0] Exit
>
    
```

4.26.3 Alarm list

This gives an overview of all alarms used. See example below:

```

Alarm list
Code      Alarm SMS      Alarm log      Alarm output      Alarm samples
PM        Disabled      Off           Disabled
RPT       Disabled      Off           Disabled
TPT       Disabled      Off           Disabled
AIN       Disabled      On            Disabled          0
MINVi     Disabled      Off           Disabled
OCi       Disabled      Off           Disabled
PTi       Disabled      Off           Disabled
CNT       Disabled      Off           Disabled

[0] Exit
>
    
```

4.26.4 Alarm limits

This gives an overview of alarm limits, used in the configuration. See example below:

```

Alarm limits
Code      Low-low Low      High      High-high      Hysteresis
PM
RPT
TPT
AIN       N/A      20        50        N/A           0.5
MINVi
OCi
PTi
CNT

[0] Exit
>
    
```

4.27 Maintenance Menu

This menu is used to perform several diagnostic tests and includes tools for the maintenance of the data logger. Below the maintenance menu is shown:

```

Maintenance

[0] Exit
[1] Field testing
[2] Comport redirect
[3] Data download
[4] Format SD card
[5] Configuration download
[6] Configuration upload
[7] Firmware upgrade
[8] Modem maintenance
[9] Bootloader menu
>
    
```

It is recommended that the user first consult this menu and run some tests, before deployment. Or, in the case of failure after proper operation, this menu has to be consulted first. The user can enter this by using either USB or remotely with TCP.

4.27.1 Field Testing

This is a very important menu which holds several test-tools. They are discussed below:

4.27.1.1 Verify Analog inputs

This feature allows the user to check the operation of the analog inputs. It shows the exact voltage, measured at the input. It shows the plain voltage / current without the addition of multipliers/offset values, that are present in the configuration. The use of this feature is to let the user check the calibration of the data logger against a well-known voltage/current source. Below a screenshot of this test is shown:

```

Verify analog inputs

Observe values refreshed every second
When finished press any key

Internal Vref = 1.2061 V (ADC = 1497)
Analog input 1 = 0.0046 mA (ADC = 0)
Analog input 2 = 0.0044 mA (ADC = 0)
Analog input 3 = 0.0043 V (ADC = 1)
Analog input 4 = 0.0070 V (ADC = 2)
Analog input 5 = 1.6498 V (ADC = 2047)

Are the analog input values OK?
Choose yes/no >
    
```

The internal reference must always be 1.2 Volts +/- 0.1 %. For using this feature in the field, just disconnect your sensor and attach your calibrator and check the value.

4.27.1.2 Digital input test

This test allows the user to test the proper operation of the digital inputs. Below a screenshot is shown:

```

Digital input test

Apply interrupts on the Digital input pin
When finished press any key

Port 1 Counter = 0

Port 2 Counter = 0

Port 3 Counter = 0
    
```

The pulses generated during this test will not interfere with your real measurements, defined in the configuration.

4.27.1.3 SD card test

Use this feature to test the SD card. There will be data written on the card, and afterwards erased. Below a screenshot is given:

```
SD card test

Data log file size = 4578 KB
Email file size    = 0 Bytes
FTP file size      = 0 Bytes
TCP file size      = 0 Bytes
Watchdog file size = 162 KB
Free disk space    = 1896 MB
File write/read OK

Press any key! >
```

The information from this test is very important. Not only the health of the SD card is tested, but also if there are some exception logged. Exceptions, where the watchdog was called to end a certain situation must NOT exist frequently. So, the size of the watchdog-file tells a lot about the operation of the system.

4.27.1.4 Battery test

This test is for evaluating the battery condition of Lithium Batteries only. The internal resistance is measured, by measuring the voltage of the cell, while increasing current consumption. A battery with an internal resistance of >1500 m ohms must be replaced.

```
Battery test

Battery voltage = 3.585 V
Battery current = 57 mA

Increasing power consumption...

Battery voltage = 3.517 V
Battery current = 157 mA

Battery resistance = 680 mOhm

Was the Battery test OK?
Choose yes/no >
```

Since the condition of rechargeable batteries changes with the state of charge, it is no use to test the batteries with this tool. Also, the internal resistance is in another region, so use this feature with lithium (LSH-20 form Saft) only!

4.27.1.5 Comport redirect

This feature allows the user to communicate with the sensor directly. It offers a transparent connection, from the USB terminal screen, to the sensor. Baud rate settings can be selected, to match the connected sensor. During the session, the sensor power switch of the data logger is enabled, to supply the sensor. So, a very convenient way of testing, troubleshooting, configuring your sensor is possible. Also comport redirect can be used for upgrading firmware of your sensor, through the data logger. The software package of the sensor can be used, after comport redirect is enabled.

The following ports are possible:

```
Comport redirect

[0] Exit
[1] Serial port
[2] Accessory port
[M] Modem
>
```

```
Port mode

[0] Exit
[1] RS232 8N1
[2] RS485 8N1
[3] SDI12
[4] RS232 7E1
[5] RS232 8E1
[6] RS232 8O1
[7] RS485 8E1
[8] RS485 8O1
[9] RS485 8N2
>
```

And the following baud rates / frame settings are supported:

4.27.1.6 Data Download

This is used to extract the logged data from the data logger, using the USB interface. (you can do this remotely, but that makes no sense, since the data logger is able to send the logged data also). The user can select 4 different file-formats: TXT, JSON and CSV (2 different versions available). The user must enter the starting- and ending date/time for the data he likes to extract. Y-modem transfer is used for data transfer data transportation. Below an example of data download is given.

```

Data download

Start date or <CR> for this day (YY/MM/DD):
Start time or <CR> for midnight (hh:mm:ss):

End date or <CR> for this day (YY/MM/DD):
End time or <CR> for midnight (hh:mm:ss):

Download data from 2016/02/02 00:00:00 till 2016/02/03
00:00:00

Data format (0 = Native(txt), 1 = CSV(.), 2 = CSV(,;), 3 =
JSON): 3

<15:37:42>
Searching...
Start record found: S;160202104917;POWER_0N;ML-315 V2.2B1

Copying...
Press <Esc> to abort copying data to output file
<15:37:46>

Select Y-Modem transfer from your terminal program menu,
to receive the data file "ML-315_.json"

Press <Esc> to abort transfer

Sending...
Data file sending OK
    
```

Afterwards, the file is downloaded on your computer.

4.27.1.7 Format SD Card

Use this tool if you like to delete all the files on the SD card, for instance when you move the data logger to a new location. It uses FAT32 to format the card, and you don't need to extract the card from the data logger. After format the card will be blank, ready for new data storage.

4.27.1.8 Configuration Down/upload

When using multiple data loggers, the configuration of them can get labor-intensive. Especially when multiple data loggers are performing the same tasks. To assist the user with configuring the loggers, configuration transfer is possible. The configuration of the data logger can be retrieved via the USB or remotely through TCP Terminal. Use YDOC-Terminal for retrieving the config from your data logger. When you like to retrieve a configuration-file from the data logger, select the option "configuration download" and use Y-modem -> receive file option. Navigate to your path of preference, and the configuration file will be downloaded to your computer. This file is a non-readable-binary file which contains all settings of your data logger. You can store this for backup-reasons or as a template to configure new data loggers.

When you like to configure a data logger with a configuration-file, select configuration upload from the menu and use y-modem-> send file for sending the configuration-file to the data logger. All settings will be applied to the logger, except the serial number (which is a static property of the data logger).

A very practical method of configuring YDOC data loggers is to use one configuration-file to configure the data logger, and afterwards personalize the logger with a unique system name.

4.27.1.9 Firmware Upgrade

Select this option for upgrading firmware. More on FW upgrade see: [Firmware Upgrade](#)

4.27.1.10 Modem Maintenance

This feature allows the testing of the modem and also supports modem firmware upgrade. This is a seldom used feature, but it is important in some rare occasions. For more info see: [Modem Firmware Upgrade](#)

4.27.1.11 Bootloader Menu

This menu is for expert-use only. It allows the user to jump to the bootloader, where the firmware is NOT loaded yet. Normally, the user does NOT use this menu or its options. Only when the logger has severe problems, this menu can help. (it is this like the old rescue disk you received with your windows computer.)

4.28 SDI-12

The **ML-2013** is provided with an SDI-12 port. This port is connected to port 2 and is shared with the normal RS232 operation. This means that the user has to select whether he wants to use RS232 or SDI-12.

The **ML-x15 and WDL-x14** (except the AD edition) is provided with an SDI-12 port as well, but it is shared with the RS-232 and RS-485 port.

When SDI-12 is selected, it acts like a SDI-12 recorder and its specific SDI-12 commands are embedded in the driver of the input-sensor. So, the user can easily select his sensor and specify its SDI-12-address. For more information see the description of your SDI-12 sensor.


4.28.1 SDI-12 Hardware

The SDI-12 standard is a very commonly used interface-standard. The signal levels are quite different from those of RS232 and RS485. So, you cannot connect a SDI-12 sensor to a RS232 or RS485 port, it won't work. The use of converters between RS232/485 and SDI-12 is discouraged, because of the high pricing of the converters and the bad performance (see note).

4.28.2 SDI-12 Wiring

The SDI-12 electrical interface uses the SDI-12 bus to transmit serial data between SDI-12 data recorders and sensors. The SDI-12 bus is the cable that connects multiple SDI-12 devices. This is a cable with three conductors:

- 1) a serial data line, 2) a ground line and 3) a 12VDC line

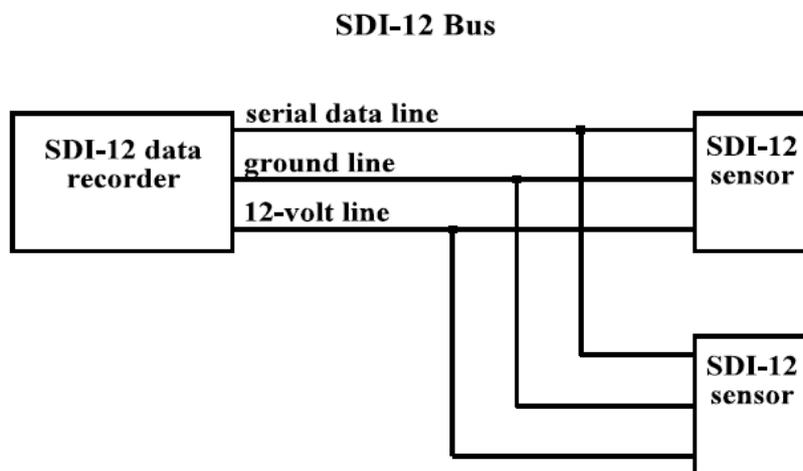

The wiring length between a sensor and the data-recorder must not exceed 60 meters. The maximum number of sensor connected to a SDI-12 bus is limited to 10. The data logger is protected against transients on the SDI-12 bus.

4.28.3 SDI-12 Baud Rate and Frame Format

The baud rate for SDI-12 is 1200. Frame format is as follows:

- 1 start bit
- 7 data bits, least significant bit transmitted first
- 1 parity bit, even parity
- 1 stop bit

Note:

SDI-12 is a half-duplex protocol, so the data-recorder has to switch between transmitting and receiving. A convertor from RS232 ⇔ SDI-12, must perform this task. However, it is not aware of the exact timing of the protocol. Therefore, it uses fixed (or configurable) delays to switch between TX and RX. After each byte send by the convertor, it waits, during the fixed delay, for another character, and if it doesn't arrive, it switches to RX. The intelligence needed to perform these tasks is mostly done by a microcontroller inside the convertor, that's the main reason for its high pricing. This method is doing the job for most cases, but it is not as good as a real SDI-12 port. The real SDI-12 port is aware of the exact protocol-timings and after the last character it switches to RX-mode immediately, without the delay. Therefore, no replies are missing. Your YDOC data logger has a true SDI-12 port.

For more information on the SDI-12 protocol: see www.sdi-12.org

4.29 RS232

Your data logger comes with 1 or 2 RS232 ports, capable of baud rates of up to 115200 bps (230400 bps on request). The ports are: port 1 and port 2. Port one is shared with the RS-485 port and port 2 is shared with the SDI-12 port. The user can choose any combination he likes, as long as he is using only one at a time. (e.g. you cannot share RS232 and RS485 one the same port). If a user needs RS232 and RS485 simultaneously, he needs to setup Port 2 also.

The ML-215/315 (except the ML-x15AD) comes with one RS-232 port, which is shared with SDI-12 or RS-485

RS232 is a widely spread interface standard, which uses 3 wires (minimum) for data communication. It is a so called asymmetric interface, that uses one wire for TX, one for RX and one for ground. It is called asymmetrical, because it uses only one wire per signal. Therefore, it's susceptible for interference, and hence, the maximum cable length is limited to 15meters.

Please keep in mind these limitations when you design your system.

RS232 is not a bus system, and therefore it is only allowed for one device to be connected to a RS232 port. So, the maximum number of serial devices to connect to your ML-2013 is 2. RS232 sensors should be connected to the data logger with their signals crossed. That is RX ⇔ TX.

We strongly recommend using RS485 instead of RS232, when cable length exceeds the 15m.

4.30 RS485

RS485 is a serial bus-system, which uses 3 wires for its communication. It uses a "differential balanced line", which can span relatively large distances (up to 4000 feet (1200 m)). A rule of thumb is that the speed in bit/s multiplied by the length in meters should not exceed 10^8 . Thus a 50-meter cable should not signal faster than 2 Mbit/s.

Instead of RS232, RS485 is capable of communicating with more than one device. After all, it is a bus-system.

RS485 sensors are called "slaves" and must have their unique address. The data logger acts as a master and retrieves the information from the slaves. Only one slave can respond to the requests of the master at a time.

To set up your RS485 sensor for use with the data logger, make sure that the address is programmed correctly, and that the sensor address is unique.




Figure 1: RS485 Wiring

RS485 is often used with MODBUS/RTU-sensors, and is less susceptible for Electrical interference than RS232.

Your data logger has one RS485 port which is capable of driving multiple sensors (maximum number of sensors depends on specs from the manufacturer of the sensor, a practical figure is 10. The maximum number of slaves, defined by EIA/RS485 is 32). For the exact number of sensors, you can connect to your ML-2013 see chapter [Firmware Driver limitations](#)


We recommend using twisted pair cable to connect to the sensors.

4.31 Analog Inputs (4..20mA)

The ML-2013 is equipped with four and the ML-x15/WDL-x14 (except the DS edition) with two analog mA 12 bits AD-Conversion inputs. The input signal must be a 4..20 mA current loop. The impedance of the system is 150 ohms.

4.31.1 Loop Powered Devices

Some devices don't need a power supply, but take their power from the current loop. But the primary circuit of the data logger does NOT provide power for this. In this case, you need the power switch to provide the energy for the current-loop. Consult the manual of the loop-powered device you like to connect, and use the positive side of the power switch for the power supply. In most cases the data logger is connected to a device with an active output signal, so there will be no problems connecting it. If you have questions about interfacing your device with our data logger, contact your YDOC-dealer.

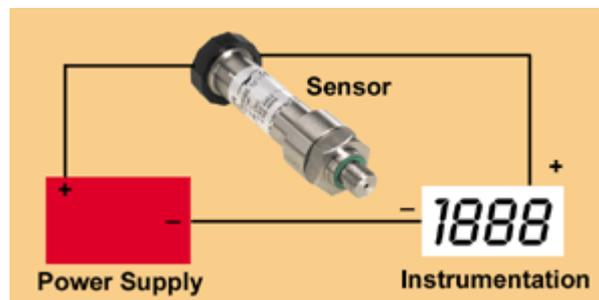

4.31.2 Analog Inputs (0 .. 10 V)

The ML-x15/WDL-x15 (except the DS edition) is equipped with two analog 0 .. 10 V 12 bits AD-Conversion inputs. The input signal must be a dc signal which must not exceed 10 Volts. The user can adopt a higher voltage level if he uses external resistors. This is done by a simple voltage divider. However this possibility offers a flexible way to expand the range of the instrument, this is NOT covered in this manual, and the user may not seek for support from YDOC on this topic.

4.32 Analog Differential Inputs (ML-2013 only)

The ML-2013 Data logger has, besides the four 12 bits analog current inputs, also two additional Differential 16 bits voltage inputs. These inputs are very sensitive and particularly suitable for measuring signals from load cells.

4.32.1 Differential input ports theory of operation

Differential inputs are very convenient for measuring differential or floating signals. The performance of a differential input is much better than a normal, single ended one, especially with small mV signals. Therefore, the differential inputs on the ML-2013 are very suitable for measuring load cells, pyranometers and other low-level mV output sensors. A differential input consists of a negative (-) and a positive (+) input. The voltage difference between these two inputs is the signal to be measured.

4.32.2 Common mode noise rejection


One of the major advantages over a single ended input is the common mode noise rejection. It "removes" practically all noise that is present on the input signal. Especially with long cables, noise is always present on the leads. Since the input acts like a differential amplifier, the noise on the negative input is subtracted from the noise on the positive input. What is left is the sensor-signal.

4.32.3 Using Load Cells With the ML-2013

The ML2013 is very suitable for connecting load cells and other resistive elements. A load cell acts as a bridge of Wheatstone and is a very sensitive and precise passive component.

4.32.4 Bridge of Wheatstone

The bridge of Wheatstone (the principle of operation of a load cell) is a circuit, consisting of 4 resistors. Below a circuit is given:

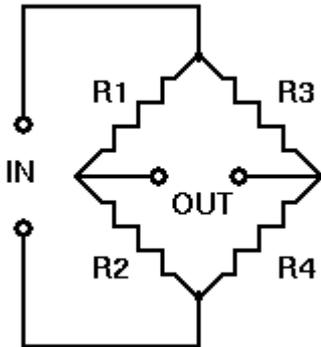

Given, all R's are the same the output voltage will be 0 Volts. In practice, one of the resistors is replaced by a variable resistor (often a strain gauge). By varying the resistance of this resistor, the bridge will be "unbalanced" and there will be an output Voltage, other than 0 Volts. To enable the circuit, the bridge has to be powered by a very stable reference Voltage, often called "Excitation Voltage". The ML2013 has an Excitation output for this purpose.


4.32.5 Excitation Output.

The ML-2013 has an Excitation output for powering load cells, or other devices. It is a single output with a fixed precision voltage output. This Excitation output is driven by the Power Switch of the ML-2013. The default, fixed, Excitation Voltage is 5.000 Volts. For most load cells, this is OK. However, if the user wishes another value, it can be selected by selecting 3 soldering jumpers on the bottom side of the board.

Here is how to set the jumpers for the correct Excitation Voltage:

Excitation Voltage Configuration			
SJ1	SJ2	SJ3	Voltage
Open	Closed	Open	2.500 V
Closed	Open	Open	5.000 V
Open	Closed	Open	7.500 V

The default excitation is 5.000 V

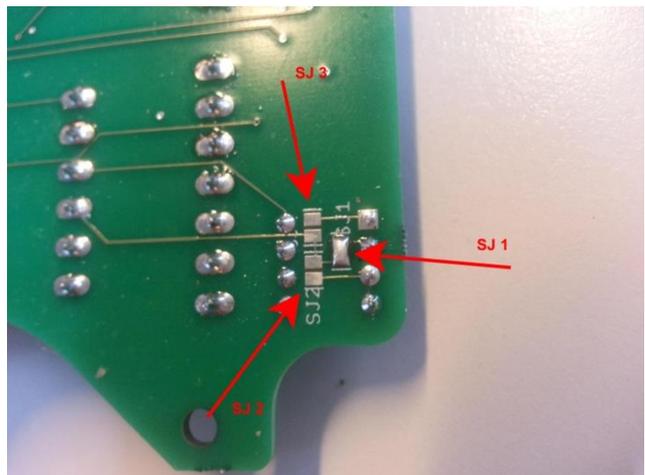

4.32.6 Analog Differential input 5

Analog input 5 is a Differential input with a build-in user selectable input-amplifier. Therefore channel 5 has a user selectable range. The user can set the range of the input according to his preferences. This is done by adjusting the so called “port mode” The Ranges are given in the table underneath:

Input 5 ranges	
Port mode	Voltage
0	0 .. 250mV
1	0 .. 500mV
3	0 .. 1000mV
4	0 .. 2000mV

4.32.7 Analog Differential input 6

Analog input 6 is the most sensitive differential input of the ML-2013. With exception of this sensitivity, the channel is similar to channel 5.

Input 6 ranges	
Port mode	Voltage
0	0 .. 10mV
1	0 .. 20mV
3	0 .. 40mV
4	0 .. 80mV

4.32.8 Calibration of Differential inputs

The Differential inputs are calibrated at the factory. This calibration is a so called 1 point zero offset calibration. With this type of calibration, only the value at zero is adjusted. For input 5 this is very accurate, it will be < 0.05 %. For an application that requires an even higher accuracy, the user can and should do a user – overall calibration.

4.32.9 Overall Calibration

This type of calibration is offered to the user to get the most accurate readings possible. This type of calibration is a two-point’s calibration.

How it works:

The user can enter 2 pre-defined data values into the ML2013. This is very convenient for i.e. Scales. For example, the user has a standard load of 1 kg and one of 10 kg. He starts the calibration procedure, and starts with the 1.0 kg load. The data logger, now, adapts the 1 kg and stores this value. Again, with the 10.0 kg load, it adjusts the scale to 10.0 kg and stores the settings. Now, the logger will calculate a linear function between the two points. Note that all deviations in the sensor or the load are compensated from now on. With this type of calibration an accuracy of < 0.01 % is possible.

Note: for Channel six, with the enhanced pre-amplifier, this overall calibration is a must do. It is not sufficient to only use the factory calibration. The factory calibration for this input is < 0.5%.

4.33 Potentiometer input

The ML-x15/17 (except the DS edition) is equipped with a potentiometer input. This input is a 0..3300mV voltage input. It is designed especially for potentiometers, like the ones in winddirection meters and angle meters. This input is connected to the internal ADC directly and is translated into a 0 % - 100% value. The user has to connect the potentiometer between the 3.30V Vref and ground. The ML-x15/17 models have a Vref output for that. (Terminal X1.8). Because of the fact of the potentiometer is connected between Vref and ground, the ADC value will always be the full range (0..4095) INDEPENDENT of the value of the connected potentiometer. So, all types and all values of potentiometers are supported.




Although all values are supported, we strongly recommend to use high values only. This is because the lower values are draining more power from the data logger. Values between 100K and 4M Ω are recommended.

A potentiometer gives a value what is translated to 0.. 100%, and can be re-scaled to engineering values by the user. A potentiometer is a variable resistor with three terminals. (see picture below)



Figure 2: Potentiometer

The two outer terminals are connected to the fixed resistor and the middle terminal is connected to a slider. So, when a potentiometer is turned, the resistance between the middle terminal and one of the outer terminals is changing with the angle of the potentiometer. Very often potentiometers are used to regulate a voltage from 0% to 100 % of the input voltage. In the next figure this well know circuit is drawn.



The output voltage is adjustable from 0% to 100% of V_{in} , in this case. The ML-x15 data logger has 3 terminals (on connector X1) for connecting a potentiometer to the logger:

X1.6 = GND

X1.7 = 0..100% Resistance

X1.8 = Resistance Reference terminal

So, the circuit above is connected as follows:

IN+ = X1.8

GND = - = X1.6

OUT = X1.7

Another application of the use of the potentiometer-input is to connect a PT-1000 temperature sensor to the potentiometer-input. In the appendix is this example explained



The resistance reference terminal is derived from the internal ADC reference and has a 150-ohm series resistor (to prevent damage in case of a wiring fault). The internal reference has a level of 3.30 Volts. When relative low impedance potentiometers are used, there will be a voltage drop across the internal series resistor, and the max ADC value won't be reached. Another reason to use only high impedance potentiometers. Of course, when a sensor has got a low impedance value, you can use it, but you have to compensate for the voltage-drop.

4.34 Digital inputs

The **ML-2013** is equipped with 4, the **ML-x15/x17** with 3 and the **WDL-x15** with 1 digital input(s). These inputs are interrupt-driven what means that they activate the data logger to wake up when sleeping, and that a signal-change on the input is never missed. So, these inputs are ideal to use for counting events (like the pulses from an energy-meter or a rain gage), or to set an Alarm state (e.g. level or float switch). The signal level needs to be zero volts and 3.6 volts (“0” level and “1” level). The inputs are “5 Volts tolerant” So standard 5 Volts signals are also OK. Any other voltage needs to be adapted to the right range, before connecting. The user can select whether the input has to be “pull-up” or “pull down”

4.34.1 Pull up type

The pull up type of input means that there is an internal resistor (40 K) mounted between the input and the Vcc Power supply. So, when NO signal is connected, the input will be logical high. This type of inputs is very convenient for use with “[open collector](#)” systems or “NPN outputs”

4.34.2 Pull down type

The pull up type of input means that there is an internal resistor (40K) mounted between the input and the ground. So, when NO signal is connected, the input will be logical low. This type of inputs is very convenient for use with “active output” systems or “PNP outputs”

4.34.3 Electrical specifications Digital inputs

Below table give an overview of the Electrical specifications of the Digital inputs

Vil is logical low level

Vih is logical high level

Pull up/ down resistors are 40 k typical.

Parameter	Min	Max
Vil	0V	1.25V
Vih	1.67V	5 V
Impedance	30K	50K

4.35 Coil input

Input #4 (**ML-2013 only**) is a special digital input. It is a so called “coil input”. This is a very sensitive digital input. From point of functionality, the input is exact the same as the other inputs, but electrically there are differences.

While the normal digital ports use the 0, 5 Volts levels (or 0, 3.6 Volts) the coil input uses very low signal levels, of only a couple of mill volts. This input is used for devices with this “energy less” system.

Attention: The coil input of the ML-2013 is so sensitive that a short piece of unconnected wire is enough to let the ML-2013 “pick up” signals from the environment. Be aware of this, and use a shielded cable. The reception of RF-signals can lead to problems with the performance of the system. The coil-input can demand very much processing power, in case of reception of RF-signals.



The coil input is very convenient when used with water meters with a passive coil output.

4.36 Alarming

In some circumstances, normal data-logging is not sufficient for managing your process. For keeping track of certain, often critical, conditions, the data logger is equipped with direct alarming options. Alarming-limits and hysteresis are used to manage these special events. The table below shows the different types of alarming-limits.

Alarm Limit	Description	Remarks
Low-Low	Alarm level for lowest value	This alarm level is reached when the data logger encounters a value which is lower than the low-low Limit, this is the 2nd and most urgent state of alarming. This type of alarming is used for very rare and critical conditions. (often called STOP level)
Low	Alarm level for low value	This alarm level is reached when the data logger encounters a value which is Lower than the Low Limit, but Higher than the Low-Low Limit. This is the first stage of alarming. (often called WARNING level)
High	Alarm level for high value	This alarm level is reached when the data logger encounters a value which is higher than the high Limit, but lower than the High-High Limit. This is the first stage of alarming. (often called WARNING level)
High-High	Alarm level for highest value	This alarm level is reached when the data logger encounters a value which is higher than the high-high Limit, this is the 2nd and most urgent state of alarming. This type of alarming is used for very rare and critical conditions (often called STOP level).

4.36.1 Alarming - principal of operation


When a data logger is running, and a measurement is out of boundary, the data logger will immediately switch over the alarm sample interval. So, the first-time a –out of boundary-value will be detected is at the normal data-log interval and from this moment on, the data logger will increase its sample interval to the alarm-sample interval. The “alarm sample delay” determines what happens next. If this value is equal to zero, action is taken immediately. If the sample interval delay is 1, the logger will wait for one more alarming cycle upon taking action. If the alarm interval delay is 2, it will take 2 cycles, etc.

When this alarm-state is entered, the data logger will add the ‘*A’ data modifier to the data-records. The user has the following options for the requested action:

- 1) Alarm log (log an alarm level)
- 2) Alarm message (SMS, E-mail or MQTT)
- 3) Direct log data output on alarm (HTTP, E-mail, FTP, TCP or MQTT)

So, when the conditions of alarming are met (data value out of bounds and the alarm sample delay is expired) one or more of these actions can take place.

Note: The alarm log is a log of synoptically data into an S-record. The data modifier *A is automatically placed into the D-records.

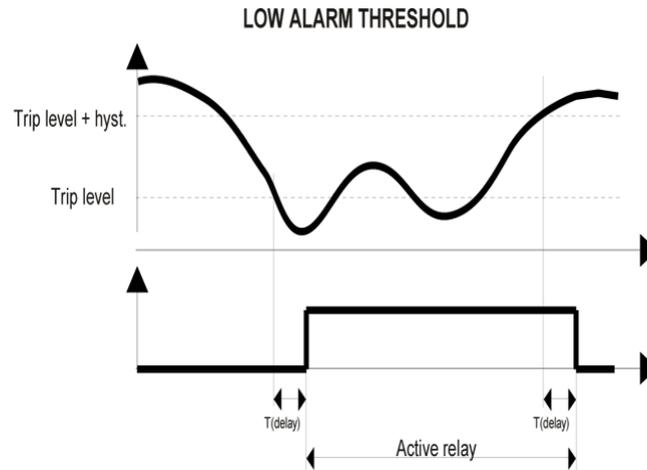

So, the entry of an alarm state is NOT affected by a hysteresis. Hysteresis is only used for switching back to the normal mode. The amount of hysteresis has an effect on the “sensitivity” of the alarming. It is strongly advised to use a certain amount of hysteresis to prevent from multiple alarming warnings. The amount of hysteresis is determined by experience and information from the sensor.

4.36.2 Advanced Alarming

From firmware-version V2.1B1 and above, we implemented an extended alarming feature that enables the use of calculated channels. This feature was implemented to calculate meaningful engineering values derived from raw sensor input values, however they could also be used for advanced alarming using multiple input conditions. It was already possible to raise an alarm (SMS or trigger a digital output) on exceeding of configured limits for a single input value (e.g. alarm to warn for reservoir overflow). By using calculated channels, it is now possible to alarm on a combination of input values.

Example:

Assume an open water reservoir for irrigation purpose and you want to be warned when the water in the pond falls below a certain level or when the water level reaches the edge of the reservoir. But why ring any bells if the pond level is just falling below the warning level (due to vaporization) while there is no demand for water or why alarm when water is just over a high limit (due to precipitation) while there is no forced supply.

To avoid unnecessary level alarms, you could define a calculated channel with the following equation:

$$\text{ALARMLEVEL} = \text{gt}(:\text{FLOWIN}; 0; :\text{LEVEL}; \text{gt}(:\text{FLOWOUT}; 0; :\text{LEVEL}; \text{LEVELOK}))$$

Where:

gt(a; b; c; d) is a function that returns the value c when a>b otherwise it returns d.

:FLOWIN is the monitored supply flow or a digital switch indicating an open valve/floodgate

:FLOWOUT is the monitored demand flow or a digital switch indicating an open valve/floodgate

:LEVEL is the monitored level in the pond

LEVELOK should be substituted by a level value that does not ring any bells, a pond level somewhere between low and high limit.

ALARMLEVEL is the defined calculated channel, which will be set to the same value as :LEVEL when there is a supply (:FLOWIN > 0) or demand (:FLOWOUT > 0) flow, else it will return a level that does not ring any bells (LEVELOK value).

Instead of setting low/high limits to :LEVEL you should set the warning limits to the ALARMLEVEL channel.

For safety reasons you could still set low-low/high-high limits to :LEVEL.

4.37 Firmware Upgrade

The data logger is equipped with a boot loader, which enables the firmware upgrade feature. Firmware upgrading allows a user to overwrite the internal firmware of the data logger with a (newer) updated version of the firmware. Firmware upgrading can be done by using:

- USB connection
- Wireless via 2G/3G (TCP, HTTP or MQTT)
- Via Comport

4.37.1 When to use Firmware upgrades

Normally, a user never uses this feature, as long as he is satisfied with the performance of the system. In time however, the need for additional features may arise. For example, a new serial sensor is introduced on the market and a customer wants to connect this sensor to the data logger. When YDOC has extended the firmware to support that sensor, a new version of the firmware is released. After the user has performed the firmware upgrade, his “old” data logger, now supports the new sensor. Normally, when the system is running fine, and no additional requests exists, we recommend NOT to perform a firmware-upgrade.

4.37.2 Firmware upgrade procedure

How to perform a firmware upgrade:

- First download the latest version of the firmware from your YDOC-Dealer.
- Download the ydocTerminalYDOC Terminal setup from <http://your-data-our-care.com/data-logger-utilities.html>
- Use the menu and select the option “Maintenance”.
- Follow instructions from the menu.
- Use “Y-Modem protocol” to send the new firmware to the data logger.
- Don’t remove the USB nor power from the data logger
- When these steps are completed, the new firmware is active.

We recommend the use of the USB-connection over the wireless function. This is because of possible drop outs in communication. When a firmware upgrade procedure is interrupted, the upgrade will fail, but the unit continues to operate, with the previous version. The USB- connection is faster and more reliable.

4.37.3 Firmware upgrade over the air

It is also possible to perform a firmware upgrade over the air. This can be done by ydocTerminal in combination with YDOC Java TCP-server or ydocInsights data collector. It can also be performed by ydocTerminal in combination with an MQTT-broker or by HTTP from your webserver.

4.37.4 Firmware Driver limitations

The data logger is equipped with various drivers, for several tasks. The number of total drivers is limited to 16. This means you can choose maximum 16 drivers from all the drivers available. Each driver can handle (collect or send) a number of parameters. The total number of parameters is limited to 64. So, theoretically, the data logger can handle up to 16 sensors with each 4 parameters. But in this case, there is no output possible. In most cases two or three drivers are needed for minimum operation (internal driver, tcp output-driver, or email-driver). When a user has an additional analog sensor, it will take a driver as well.

Example:

A user wants to connect a large number of INW CT2X sensors to an ML-2013. This sensor measures temperature and conductivity. So, each sensor “uses” two parameters. Also, he likes to send the data via FTP, and he enables the following internal sensors: Rest Capacity, Battery Voltage, and Current. So, besides the Sensor drivers there are 2 drivers needed:

- Internal Driver
- Output Driver

So, the maximum number of Sensor-drivers is: $16 - 2 = 14$

So, there are 14 Sensor-drivers left for use with the CT2x sensors.

The total number of parameters is: $14 * 2 + 3 = 31$

So, the number of parameters is no problem ($31 < 64$)

He can connect 14 CT2X sensors max.

4.37.5 Power Switch Limitations

The Power Switch is capable of powering sensors up to 100 mA. The output voltage is 12 Volts DC.

4.37.6 Modem

The modem inside the ML-2013, ML-215, ML-217 and WDL-214 is capable of GPRS and GSM communications. It has quad band support, so it can be used worldwide. For selecting the proper frequency band, use the “modem settings” in the configuration menu. In most cases GPRS communication is requested, so use a GPRS enabled SIM-card to inhibit this operation. Consult your local telecom provider for the right SIM-Card and – settings. If GSM communication is requested, use a GSM-DATA subscription. GSM communication is suitable for modem dial in communication. We strongly advise to activate this option in the SIM cards used in the logger. This is often used to re-configure a logger, remotely, or to monitor actual values. In most cases, normal GPRS communication is sufficient for the operation of the data logger.

The modem inside the ML-315 and WDL-314 is capable of 900MHz/2100Mhz 3G communication as used in the EMEA and APAC regions.

The modem inside the ML-N315, ML-317 and WDL-N314 is capable of 850MHz/1900Mhz 3G communication as used in North American regions.

4.37.7 Modem Firmware Upgrade

The modem inside the data logger is equipped with the latest firmware-version available. There is no need for upgrading the software, even in the near future we don't expect this to be needed. But just in the unlikely event of the need of a modem firmware, it is possible to do so. This can be done with the modem mounted on the board (in circuit programming). The procedure of upgrading modem firmware is not covered in this manual. For more information, consult your local YDOC dealer.

4.38 SD-card

The SD-card used with the data logger is a SANDISK 2GB/4GB type Card. It is formatted in FAT 32, and is compatible for use with a PC. Don't use other cards than this type, because the performance of the data logger may be harmed. (This is because of the speed of the SD-card, and even the low power performance can be affected by using a slower card). The contents of the card may be read on a PC by using a card adaptor, or can be downloaded from the card, by using the menu-option “Data-download”. We recommend not removing the SD-card from the logger.

4.38.1 Inserting an SD-card

At the factory, the SD-card is already installed, but when the cards need to be re-inserted, pay attention to the orientation of it. It should be inserted with the (gold-plated) terminals up.

4.39 Native TXT Data Format

The log file data format uses different records for data output. There are two types of data records:

- D-records
- S-records

4.39.1.1 Header:

In every log file, first a header is transmitted. This header contains all information about the data following in the next records. The syntax of the header is;

```
<'L'> <'> [ <Parameter Code> <'> < Parameter Name > <'> < Parameter Unit> <'> ]
```

This means that the line starts with an 'L' character, followed by a semicolon. Then the code, name and unit of the parameter follow. These last 3 elements must be repeated for each logged parameter.

```
L;RCi;Rest Capacity;%;PTi;Processor
Temperature;C;Vi;Voltage;V;AVGCI;Average Current;mA;0Ci;0perating
Cycle;sec;S%;GSM Signal;%;MAXCI;Max Current;mA
```

Example header:

So, the header consists of these elements:

1. L
2. Parameter Code
3. Parameter Name
4. Parameter Unit
5. ;

4.39.1.2 Parameter Code:

The abbreviation of the full parameter name, it may be up to 7 characters long.

4.39.1.3 Parameter Name:

The name of the logged parameter, it may be up to 31 characters long.

4.39.1.4 Parameter Unit:

The unit representing the physical dimensions of the measurement, it may be up to 15 characters long.

All characters are allowed except ';' this is reserved for a separator.

4.39.2 D-Records

Most of the data is logged into D-records. D-records stand for Data records. The syntax of this record is;

```
<'D'> <'>,<Timestamp> <'> [ <Parameter Code> <'> < Parameter Value >[<Data Modifier>] <'>]
```

So, the D-record consists of a 'D' character followed by a timestamp, and after that, one or more series of parameter code and parameter name. So, the D-record consists of these elements:

1. D
2. Parameter Code
3. Parameter Value
4. Optional Data Modifier
5. ;

4.39.2.1 Parameter Code:

The abbreviation of the full parameter name, it may be up to 7 characters long.

4.39.2.2 Parameter value:

The numeric value of the measurement, together with an optional data modifier, forms the measurement.

Example Data-record(s):

```
D;110928030200;RCi;95.8;PTi;50.1;Vi;3.6;AVGCI;71;0Ci;0.25;MAXCi;71
D;110928030300;RCi;95.8;PTi;49.3;Vi;3.6;AVGCI;71;0Ci;0.25;MAXCi;72
D;110928030400;RCi;95.8;PTi;49.5;Vi;3.6;AVGCI;72;0Ci;0.25;MAXCi;72
D;110928030500;RCi;95.8;PTi;49.1;Vi;3.6;AVGCI;72;0Ci;0.25;MAXCi;54
D;110928030600;RCi;95.8;PTi;49.1;Vi;3.6;AVGCI;54;0Ci;0.25;MAXCi;72
```

4.39.3 System records

The System-records are used to log system related information. System-records do not contain normal measurements. A system-record is made, when a deviating situation has occurred, for instance, when a sensor is not replying to a request from the logger. System-records are used for monitoring system-performance.

The syntax of an S-record is:

```
S;<Timestamp>;<Message code>[;<Supplemental code or text;["<Explanatory text>"]]
```

So, the S-record consists of an 'S' character followed by a timestamp, and after that, one or more series of parameter code and parameter name.

So the S-record consists of these elements

1. S (to distinguish a system record from a data record)
2. Timestamp (yymmddhhss)
3. Message code
4. Optional supplemental code or text
5. Optional explanatory text

See Appendix 'System messages' for a list of possible messages and their meanings.

Example S-records:

```
S;110922202054;CFG_RESET
S;110922202054;CFG_CHANGED;Brasil_3002389
S;110922202124;MODEM_WDT;STATE 10
```

4.39.4 Data Modifiers

Normally a data value, presented in D-records is recorded without a Data Modifiers, but in case of a malfunction, or rare circumstances, a Data Modifier is added to the data value. See table below:

Data Modifier	Description	Remarks
*T	Timeout	The sensor did not provide the data logger with a data value, and the timeout has expired. The previous data value is recorded, with the addition of this exception.
*I	Data Invalid	The data logger did receive a data value from the sensor, but it was out of boundary. This exception is very rare.
*A	Alarm Value	The data logger has received a value, which is outside the limits of the particular parameter.

4.40 JSON Data Format

The JSON Data Format contains about the same info as our native TXT data format, but formatted in JavaScript Object Notation (JSON) format. This format is preferred by web developers as the data can be easily accessed by JavaScript or other scripting languages like PHP. When using ydocInsights we recommend using our native TXT format as it has lesser overhead resulting in lower data payload (costs) and data transfer time (power consumption).

The JSON object contained in the file exists out of three main objects:

- 1) The **“device”-object** is having three variables:
 1. “sn” a string giving the unique serial number of the logger.
 2. “name” a string giving a user chosen name for the data logger.
 3. “v” a string giving the version of the Firmware

```
"device":{"sn":5152860,"name":"Demo 1","v":"2.2B2"},
```

- 2) The **“channels”-object** is an array of objects listing all configured data log parameters, each channel/parameter object is having 3 variables:
 1. “code” a string specifying the Parameter’s user defined code, e.g. PTi
 2. “name” a string specifying the Parameter’s user defined name, e.g. Processor Temperature
 3. “unit” a string specifying the Parameter’s user defined unit, e.g. °C

```
"channels": [
{"code":"PTi","name":"Processor Temperature","unit":"°C"},
{"code":"CHx","name":"Channel x","unit":"Unit x"},
{"code":"SB","name":"Signal quality","unit":"bars"},
{}],
```

The “channels” array is, for convenience, terminated by an empty object {}

- 3) The **“data”-object** is an array of objects listing timestamped events, a timestamped object always starts with a timestamp variable “\$ts”, followed by one or more variables, where a variable can be a logged channel value or a system (error) message. A system message variable is always identified by \$msg and a channel variable is always identified by its Parameter code (see: “channels”). Variables not being \$msg or not occurring in the “channels” array can be ignored.

The “data” array is, for convenience, terminated by an empty object {} as well.

```
"data": [
{"$ts":160225105846,"$msg":"POWER_ON;ML-215;V2.2B2"},
{"$ts":160225105900,"CHx":"0*T", "PTi":23.5},
{"$ts":160225110000,"SB":4},
{}]
```

\$ts is a timestamp formatted as a number yymmddhhmmss

\$msg is a string giving some system message (See Appendix ‘System messages’ for a list of possible messages and their meanings). Other variables starting with \$ can be added in the future and can be ignored.

Variables NOT starting with \$ are considered to be logged channel variables of which the variable name should occur as “code” in the “channels” array.

A channel variable can be a number (the logged value) or a string being the logged value concatenated with a data modifier. (See: 4.35.3 Data Modifiers)

4.41 Compacted Data Format

The compacted data format is meant for use in case of message size constrained or payload expensive communication, like satellite communication.

Compacting is required to get sufficient measurements in a size constrained message or to reduce expensive payload costs.

A common method to compact data is by using algorithms like “zip” and “rar”, but those algorithms are not suitable to compress size constrained messages and would make the payload rather bigger than smaller.

A first stage in compacting, is eliminating data that is not strictly necessary and to include the real interesting data only. The compacted data contains timestamped measurement values only, it does not contain diagnostic data or supportive info like system identifications, parameter codes, names or units.

The compacted format is limited to contain up to 15 logger parameters/channels. As textual parameter codes would use too much data, the identification of the individual channels is based on a number between 1 and 15. Assigning the numbers to individual parameters is a matter of configuration by starting their code names with a capital P followed by a number between 1 and 15. The P will be stripped of, as well as any trailing characters, so you could specify meaning full codes like: P1TMP or P02HUM or P15LEV. Make sure that the number parts are unique.

The compacted data is a binary and unreadable format as representing times and values in ASCII format would take too much space. Storing values as IEEE floats is out of the question either, because every value would take at least 4 bytes, while less bytes would be sufficient in most cases.

The compacted data exists out of time and value records. Each record specifies the delta to the previous corresponding record. So, in case of big numbers (like with time or totalizers) only the first occurrence will take the max required bytes, while consecutive occurrence might need just one byte.

When a time record is specifying a delta of 5 minutes, all value records following will be 5 minutes younger than the ones before. When a value record is specifying a delta of 0 it means that the measured parameter value did not change since the previous measurement.

The starting reference time for each message is 1-jan-2017 00:00:00. The first record in the message will be a time record specifying the difference in time since 1-jan-2017 00:00:00 for the first value records.

The starting reference value is 0.0 for each individual parameter.

Note: The “Source” of the “Compacted Data” can be identified by the info contained in the encapsulating “Delivery Message” (e.g. the IMEI number of an Iridium Satellite Transceiver). The format and transfer method of the “Delivery Message” is dependent of the used “communication provider” (e.g. an Iridium TCP-direct message).

4.41.1 Records

A record can have a length from one to 6 bytes.

4.41.1.1 First byte of record

Bit 7	6	5	4	3	2	1	0
Type of record				Sign bit	Scaling bits		

The most significant nibble of the first byte describes the type of record, the least significant nibble its scaling and sign. See paragraphs "Time/Value-record" for more details.

The first byte is followed by 0 or up to 5 "number"-bytes.

4.41.1.2 Number-bytes

The "number"-bytes form an unsigned integer (mantissa), which can be converted to a real number by applying the scaling and sign.

Bit 7	6	5	4	3	2	1	0
Following byte bit	7-bits value * 2 ⁰ (0 to 127)						

Bit 7	6	5	4	3	2	1	0
Following byte bit	7-bits value * 2 ⁷ (128 to 16383)						

Bit 7	6	5	4	3	2	1	0
Following byte bit	7-bits value * 2 ¹⁴						

Bit 7	6	5	4	3	2	1	0
Following byte bit	7-bits value * 2 ²¹						

Bit 7	6	5	4	3	2	1	0
0	7-bits value * 2 ²⁸						

Each "number" byte contains a 7-bits value (0 to 127) and a bit to indicate that another "Number" byte is following or not. If "1" then another 7-bits value is following, which should be multiplied by 128 (2⁷) and added up to the first byte, if there is a next byte it should be multiplied by 16384 (2¹⁴) etc, etc., until the "following byte" bit is set to "0". When the "following byte" bit is "0", then a next record starts unless the end of message is reached.

Number examples:

- 00000001 = 1
- 10000001 00000010 = 1 + (2*128) = 257
- 10000001 10000010 00000011 = 1+(2*128)+(3*16384) = 49409
- 10000001 10000010 10000011 00000100 = 1+(2*128)+(3*16438)+(4*2097152) = 8438017

4.41.1.3 Time-record

Bit 7	6	5	4	3	2	1	0
Type of record=0				Sign	Single byte	Scaling value	

When the most significant nibble of the first record byte equals 0, then the record specifies a change in timestamp for all following value records.

Bit 0 & 1 indicates the scaling of the "Time"-record: 00= Day, 01=Hour, 10=Minute and 11=Second.

Bit 2, When this bit is set to "1" it indicates that there are no "Number"-bytes following this record, the record exists out of just one byte where the value equals to the scaling value (e.g. 1 day). When this bit is set to "0" the delta time is given by the value constructed from the following "Number"-bytes.

Bit 3 is the sign bit and when set to "1" it indicates that the time difference given in this record should be subtracted from the current timestamp and when "0" added to it.

4.41.1.4 Value-record

Bit 7	6	5	4	3	2	1	0
Parameter number (1 to 15)				Sign	Scaling value		

When the most significant nibble of the first record byte is unequal to 0, then the record is about a value measured at the current timestamp of a parameter with the specified number.

Note: a "Value"-record has at least one following "Number"-byte.

Bit 0,1 and 2 is a 3 bits scaling value (a value between 0 to 7). To get the real number, the integer number, constructed from the following "Number"-bytes, should be divided by 10 to the power of the scaling value. (e.g. 1= divide by 10, 2=divide by 1000).

Bit 3 is the sign bit and when set to "1" it indicates that the given delta value in this record should be subtracted from the current parameter value and when "0" added to it.

4.42 Input-drivers

Input-drivers obtain data from sensors. Various sorts of sensors can be connected to the data logger. When a sensor needs a “warm-up time” the power output switch can be used to power the sensor before the measurement is taken. The maximum time of a power delay is 5 minutes



Note:

The Power Switch output is consuming a lot of power, so try to minimize this. Consult the manual of the sensor for warm up times. A warm up time of 5 minutes is possible and can be used in rare situations, but the battery-life will be shortened enormously. In such rare cases, consult your local YDOC-supplier for a calculation of battery-life, before exploiting your data logger.

4.42.1 Analog sensors

The **ML-2013** is provided with 4 factory-calibrated analog inputs with 12 bit ADC resolution. Analog input 5 and 6 are factory pre-calibrated amplified differential inputs with 16 bit ADC resolution.

Input	Range	Accuracy	Impedance
1	4 .. 20mA	<0.1%	150 Ohm
2	4 .. 20mA	<0.1%	150 Ohm
3	4 .. 20mA	<0.1%	150 Ohm
4	4 .. 20mA	<0.1%	150 Ohm
5	0..250/500/1000/2000mV	<0.05% or <0.01%*	1 MOhm
6	0..10/20/40/80mV	<0.5% or <0.01%*	1 MOhm

To gain an accuracy of <0.01% the user should perform a two-point calibration himself, taking the whole chain into account (e.g. Wheatstone bridge and Excitation). A load cell can be calibrated by measuring it without load and with an accurate known load (e.g. a calibrated weight).

The **ML-x15/x17** (except the DS edition) is provided with 5 factory-calibrated analog inputs with 12 bit ADC resolution.

Input	Range	Accuracy	Impedance
1	4 .. 20mA	<0.1% FS	150 Ohm
2	4 .. 20mA	<0.1% FS	150 Ohm
3	0 .. 10V	<0.1% FS	32 k Ohm
4	0 .. 10V	<0.1% FS	32 k Ohm
5	Potentiometer (0..100%) or as 0..3300mV input	<0.1% FS	500 k Ohm

The **WDL-x14AD** is provided with 4 factory-calibrated analog inputs with 12 bit ADC resolution.

Input	Range	Accuracy	Impedance
1	4 .. 20mA	<0.1% FS	150 Ohm
2	4 .. 20mA	<0.1% FS	150 Ohm
3	0 .. 10V	<0.1% FS	
4	0 .. 10V	<0.1% FS	

4.42.2 Digital Pulse Sensor

Digital Pulse sensors like for instance rain gauges are based upon the “reed contact” principle. The rain gauge has an internal bucket with a very precise volume. It is constructed to tip over when it reaches a specified amount of water. The water is drained and while the bucket was turning, a magnet triggered a magnetic switch, a so called “reed contact”. So, the rain gauge itself works like a passive switch. The data logger has a special input to trigger on these events. Even when the data logger is sleeping, the event of a tipping bucket is never missed. The data logger uses a so called “interrupt-input” to make this possible. To connect a rain-gauge, use this interrupt input and connect the other site of the rain gauge to the 3V6 output.

Note:

The digital input offers the most energy-friendly measurements available. This is because the data logger is allowed to sleep most of the time, and only capture the events of the digital interrupt (e.g. the tipping bucket of a rain gauge). In the situation where only one digital sensor is used, the battery is probably going to last much longer than any other measurement. For safety-reasons a user can include some internal measurements in the configuration, to allow monitoring of the performance of the system.

4.42.2.1 Example configuration Rain Measurement

Here an example is shown for a tipping Bucket Rain Gauge, and how to set it up in the data logger. The Rain-gauge should be connected to the “Digital input”

Underneath the menu for this input is shown.

```

Digital pulse sensor

[0] Exit
[1] Name                >> Rain
[2] Sample interval    >> Data log interval
[3] Port mode          >> Port 1; Internal pull up
[4] Register mode      >> Pulse (low frequency)
[5] Units per pulse    >> 0.2
[6] Register value     >> 16979 pulses
[7] Register reset     >> Off
[8] Log each counter change >> 0n
[9] Counter (unit)     >> Counter
[A] Quantity (unit)    >> Quantity
[B] Mean rate (unit/h) >> Mean Rate
[C] Max rate (unit/h)  >> Max Rate
[D] Min rate (unit/h)  >> Min Rate
[R] Remove
>

```

First, change the name “Digital Pulse” into a more comprehensive one. We use “Rain” here. The menu-item “pulses per unit” is very important and converts the input pulses into a physical value. It is advised to test the hardware first, before proceeding to selecting the right settings for bucket-size etc. Therefore, leave this value (1) and test your sensor first.

To test, just connect it, and apply a known amount of pulses tot the data logger. You can verify this count with the command <Ctrl>A<Shift>V<Ctrl>D When this is correct you can proceed to set up your rain-gauge.

Now you have to enter the physical details of your rain-gauge.

i.e. when your rain-gauge has a tipping bucket with a size of 0.2 mm rain, enter 0.2 Units per Pulse.

You can reset the counter-value, caused by the previous test, if you like. You can do this by entering zero into the register via option 6.

If you like to automatically reset the counter-value at midnight, use option 7.

PARAMETERS

There are three parameters for using the digital input:

4.42.2.2 Counter

This is the most important parameter. It's a plain counter that counts every single pulse, and keeps on counting forever (unless you use midnight reset). The maximum count value is: 4294967295 (2^{32}) It will reset to 0 when it reaches this count.

The counter is working at all times, even at sleep mode. When the battery is replaced, this value is NOT lost, and is resuming after replacement of the battery.

4.42.2.3 Quantity

Quantity is the difference between the actual counter-value and the previous counter-value. So, when your data-log interval is set to 10 minutes, this parameter shows you the amount of pulses per 10 minutes. Every log-interval, this count is reset to zero.

Important!

So, when you use “Actual values” keep in mind that the parameter “quantity” is a running value. It will increase during the interval. And what you see at that particular moment is NOT the value that will be stored on the SD-card. This value could lead you to incorrect assumptions!!!



4.42.2.4 Rate

The parameter Rate is defined as the time between the last two pulses applied to the data logger, scaled to one hour. For rain-measurement, the parameter rate can be used for calculating "rain intensity". It allows you to differentiate a rain-shower from drizzling rain.

Example:

So, when two pulses, with a delay of 5 seconds between them, are send to the data logger, and every pulse represents 0.2 mm rain, the rate is: 1 mm per 25 seconds = 144 mm / hour



Important!

So, also this parameter is a "running value", it extrapolates the rainfall in the next hour, based upon an actual situation. So, keep this in mind.

4.43 Power supply

The data logger PCB is designed to work with a power supply of minimum 0.8 to maximum 5V DC

The ML-2013, ML-x15-LI, ML-x17-LI and WDL-x14-LI are powered with a D-size battery holder for a 3.7V Lithium cell. The ML-2013 and ML-x15 can optional be provided with a cover with integrated NiMH AA solar charger, 8..30V DC-adapter with NiMH AA charger.

4.43.1 Internal RTC backup battery

The data logger contains an internal coin cell battery to keep the internal real-time-clock running. The lifetime of the battery is at least 10-20 years, so this battery requires no exchange during the lifetime of the data logger.

4.43.2 Power consumption & Battery Life

Average current consumption @3.6V

Subject	Value	Remarks
Data logger in low power sleep	<100uA	Preferred mode of operation.
Data logger in MODEM sleep	2mA	MODEM in stand-by during SMS ACVA reception.
Data logger is awake	65mA	The logger is awake to be able to take and log a measurement.
Data logger is transferring GPRS data	220mA	Requires a good GPRS signal.

The data logger is equipped with an internal power monitor. During the active mode of the data logger, this power monitor keeps track of the power consumption of the device. When the device is going into sleep-mode, a fixed value is used to calculate the power consumption. Both are calculated and offer a fairly accurate measurement of the power consumption. Unfortunately, the behaviors of batteries are, in practice, much more complicated than the calculation made inside the data logger. So, the capacity, written on the back of the battery is only a typical value. Things like: Shelf life, ambient temperature, current draw, and peak current draw, affect the performance of the battery.


Therefore, we strongly advise to use the measurements regarding battery life as an indication only. We also recommend replacing the battery, fairly above 0%. If you want the best performance and the most optimized settings for your particular measurement location, contact the supplier of the Battery (www.saftbatteries.com). They can provide you more specific details and advise on your application. You can provide them information by sending them a bit of previously measured data, for analysis. When you have received the advice, you probably decrease the value of "Battery Capacity" in the configuration setup, to a bit lower value than the default (14 Ah)

When using the cover with integrated NiMH AA solar charger, we recommend to use LSD (long self-discharge) NiMH AA rechargeable batteries with at least a capacity of 2000mAh (e.g. GP Recyko, Sony Eneloop or Vapex Instant)

Please consult the www.your-data-our-care.com website for an online power consumption calculator.

5 Pin configuration

ML-2013

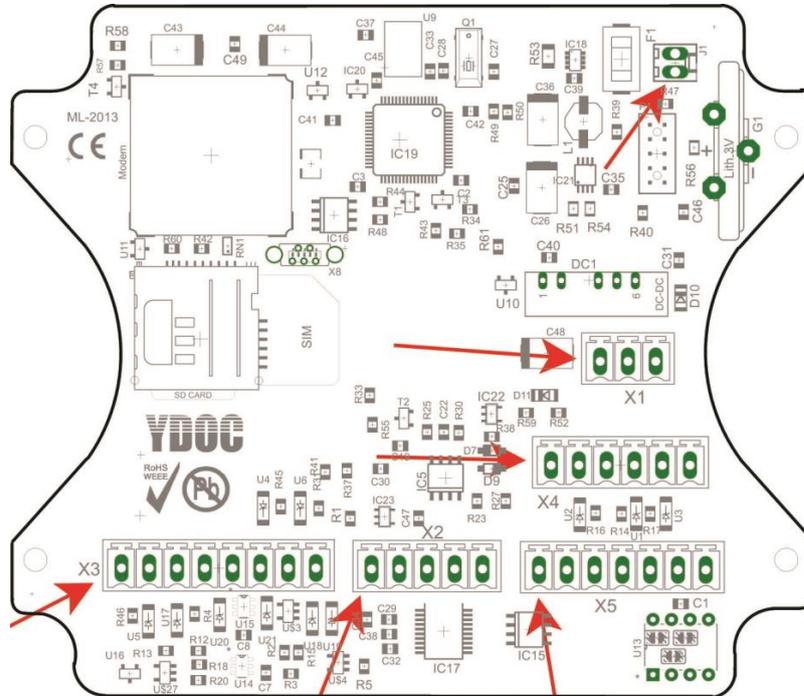

The arrows are pointing to the #1 pin

Connector	Pin#	Name	Description
X1	1	RS485 A	+RS485 positive terminal
	2	RS485 B	-RS485 negative terminal
	3	GND	Ground
X2	1	GND	Ground
	2	RS232 TX1	Transmit line RS232 port 1
	3	RS232 RX1	Receive line RS232 port 1
	4	RS232 TX2	Transmit line RS232 port 2
	5	RS232 RX2	Receive line RS232 port 2
X3	1	0..20mA input 1	Positive terminal analog input 1
	2	0..20mA input 2	Positive terminal analog input 2
	3	0..20mA input 3	Positive terminal analog input 3
	4	0..20mA input 4	Positive terminal analog input 4
	5	+diff. input 5 (0..2000mV)	Positive terminal analog input 5
	6	-diff. input 5 (0..2000mV)	Negative terminal analog input 5
	7	+diff. input 6 (0..80mV)	Positive terminal analog input 6
	8	-diff. input 6 (0..80mV)	Negative terminal analog input 6
X4	1	Switched module power output (5V)	Terminal to switch on external modules (a/o display)
	2	SDI-12 (0..5V)	Terminal to connect SDI-12 sensors
	3	Switched power output (12V @100mA)	Terminal to supply power to sensors
	4	Switched stable excitation (5V @80mA)	Terminal to supply a stable power to bridge sensors
	5,6	GND	Ground
X5	1	+coil input 4 (waveform ~50mV)	Positive terminal digital input 4
	2	-coil input 4 (waveform ~50mV)	Negative terminal digital input 4
	3	Digital input 1 (0..5V)	Positive terminal digital input 1
	4	Digital input 2 (0..5V)	Positive terminal digital input 2
	5	Digital input 3 (0..5V)	Positive terminal digital input 3
	6,7	GND	Ground
X7		ANT	U.FL connector for GSM antenna
X8		USB	USB connector for local configuration
J1	1	+VBAT (0.8 .. 5V DC)	Positive terminal for power source
	2	-VBAT (0.8 .. 5V DC)	Negative terminal for power source

5.1 ML-x15/x17



Connector	Pin	Name	Description	
X1	1	A1	0..20mA, input 1	Positive terminal analog input 1
	2	A2	0..20mA, input 2	Positive terminal analog input 2
	3	A3	0..10V, input 3	Positive terminal analog input 3
	4	A4	0..10V, input 4	Positive terminal analog input 4
	5,6	GNDs	GND	Ground
	7	PM	0..100% (0..3300mV), input 5	Positive terminal potentiometer/analog input 5
	8	PR	Reference voltage terminal	3.30V potentiometer reference terminal
	X2	1	Tx	RS232 TX
2		Rx	RS232 RX	Receive line RS232
3		A+	RS485 A	+RS485 positive terminal
4		B-	RS485 B	-RS485 negative terminal
5		SDI	SDI-12 (0..5V)	Terminal to connect SDI-12 sensors
6		GND	GND	Ground
X3	1	D1	Digital input 1 (0..5V)	Positive terminal digital input 1 or wake-up line
	2	D2	Digital input 2 (0..5V)	Positive terminal digital input 2
	3	D3	Digital input 3 (0..5V)	Positive terminal digital input 3
	4	GND	GND	Ground
X4	1	12V	100 or 200mA (ML-x17) sensor power	Terminal to supply power to sensors
	2	AO	Alarm output	Open collector (max 100mA sink current)
	3	GND	GND	Ground
X5	1	5V	600mA or 800mA (ML-x17) acc. power	To power an accessory (e.g. TFT, CAM, GPS)
	2,3	GNDs	GND	Ground
X6	4	Tx	RS232 TX	Transmit line RS232 to accessory RX
	5	Rx	RS232 RX	Receive line RS232 from accessory TX
	1		GND	USB shield GND
	2		GND	USB GND
	3		USB_data_P	Positive USB data signal
X7	4		USB_data_N	Negative USB data signal
	5		USB_VBUS	USB bus 5 Volts input
			External antenna connector	U.FL connector for external antenna
J1	1		+VBAT (3.6V DC)	Positive terminal for power source
	2		-VBAT (3.6V DC)	Negative terminal for power source
J2			Internal USB connector	USB connector for local configuration

5.2 WDL-x14



Connector	Pin#	Name	Description
X1		Internal USB connector	USB connector for local configuration
X2		UF.L connector	To connect UF.L antenna signal cable to main pcb
X3	1	GND	Ground
	2	Alarm output	Open collector (max 100mA sink current)
X4		Flex cable connector	Power and data signals to main pcb
J1	1	+VBAT (3.6V DC)	Positive terminal for power source
	2	-VBAT (3.6V DC)	Negative terminal for power source



Connector	Pin#	Name	Description
X1		Flex cable connector	Power and data signals from antenna pcb
X2		Flex cable connector	To Hirschmann 7-pole female connector
Hirschmann DS edition	1	n/c	
	2	n/c	
	3	RS-232-TX or RS485-A or SDI-12	Transmit line RS232 or RS-485 positive or SDI-12 (0..5V)
	4	RS-232-RX or RS485-B	Receive line RS232 or RS-485 negative
	5	Digital input 1 (0..5V)	Positive terminal digital input 1
	6	GND	Ground
	7	Switched power output (12V@100mA)	Terminal to supply power to sensors
Hirschmann AD edition	1	0..20mA, input 1	Positive terminal analog input 1
	2	0..20mA, input 2	Positive terminal analog input 2
	3	0..10V, input 3	Positive terminal analog input 3
	4	0..10V, input 4	Positive terminal analog input 4
	5	Digital input 1 (0..5V)	Positive terminal digital input 1
	6	GND	Ground
	7	Switched power output (12V@100mA)	Terminal to supply power to sensors
X3	1	UF.L connector	To connect UF.L cable to antenna pcb

Pin description

5.3 Pin descriptions

5.3.1 Analog Inputs

5.3.1.1 0/4..20mA inputs

Analog Input 1 to 4 (ML-2013) or 1 to 2 (ML-x15AD/ADS/TFT, ML-x17AD/ADS/TFT, WDL-x14AD)
These are Current-inputs, with an input impedance of 15 ohms. The range is 4 .. 20 mA. The circuits are equipped with over current-protection. To use this input connect the + of the sensor to the + of the power switch and the – of the sensor to the analog input pin.

5.3.1.2 0...10V inputs

Analog Input 3 to 4 (ML-x15AD/ADS/TFT & ML-x17AD/ADS/TFT only)
0..10V single ended

5.3.1.3 Potentiometer input

Analog Input 5 (ML-x15AD/ADS/TFT & ML-x17AD/ADS/TFT)
Resistance 100K to 4M7 potentiometer type recommended / 0..3300mV single ended
Analog Input 5 to 8 (ML-2013 only)
These are differential voltage-inputs, with an input impedance of 1 MOhms. The max. range is 4 .. 2000mV.
To use this input connect the + of the sensor to the + input and the – of the sensor to the – input.

There are some terminals which hold ground level, This provides both sensor-ground and battery ground. For your convenience, these terminals are connected to multiple pads on the connector PCB, because every single sensor will need his own ground. You can connect multiple sensors. When more connections are needed, just connect a wire from there and put the additional connections in parallel.

5.3.2 RS485 A & B

These are the pins for RS485 communication. Use these pins together with a ground signal. These signals are ESD-protected by the driver-circuit. The signal levels are according to the *TIA/EIA-485* Standard.

5.3.3 Power Switch

This is an output to drive one or more sensors. It holds a level of 12 Volts and is capable of driving up to 100 mA.

5.3.4 VBAT +

This is the main power supply input for the board. The level is 3.6 Volts.
Note: This signal is NOT the same as the internal 3.6 volts level. The power-supply circuit converts this level to the fixed, internal, 3.6 Volts level. This voltage level is allowed to be between 0.8 volts and 5 Volts. We strongly recommend using a 3.6 Volts Power source only. The actual voltage on this pin is monitored by the firmware. It is called "Primary input Voltage". Also the current, flowing through the 2 wires, is monitored, and is called "Primary input Current".

5.3.5 RS232 RX & TX

These are the pins for RS232 communications. Use these pins together with ground. All pins are protected against ESD. Voltage levels are according RS232 standard.

5.3.6 SDI-12 Hi

This is the in/out terminal for SDI-12 communication. It is protected against overvoltage. Use this terminal together with ground. See www.sdi-12.org for more information.

5.3.7 Digital inputs

These are interrupt-driven inputs, with an internal pull-down or pull-up resistor. To use it, connect a switch between the 3V6 or the GND respectively and this terminal. It is suitable for energy meters, water meters and rain-gauges.

5.3.8 +3V6

This is a power output. It is used to power external sensors or a potentiometer. It has a voltage of 3.6 Volts and is capable of driving up to 100 mA.

5.3.9 Antenna placement and field strength

An antenna is required for 2G/3G/4G and GSM operation. Normally you will require a dual-band antenna suitable for 900&1800 MHz or 850&1900MHz.

Depending on local field strength the integrated antenna or a simple whip antenna direct connected to the data logger will work, or a better antenna and/or better antenna placement might be required.

You can monitor the actual field strength through the configuration software(menu). The field strength may vary on atmospheric conditions, so we recommend you to make sure that the indication is maximized at installation

The field strength may also vary on the growth of vegetation (trees tend to block the signal). We also recommend configuring the data logger in such a way that the 2G/3G/4G field strength is recorded during data transfer. In this way you can get an early warning when the field strength gets low.

What to do to get a better field strength signal;

- Make sure the antenna is mounted in accordance with the manufacturer's instructions. Note there are antennas (whip antennas) that require a metal surface below the antenna; others (dipole antennas) do not.
- Make sure that all connectors on the antenna and antenna cable are tightened and free of moisture.
- Make sure the antenna is in vertical position; as the GSM and 2G/3G/4G radio signals are vertically polarize, the antenna should be vertical positioned for maximum performance.
- Do not place the antenna near metal surfaces or structures. Be aware that various building structures contain metal (e.g. steel mesh as reinforcement for concrete).
- Place the antenna outdoors.
- Identify the nearest GSM tower of your provider. Place the antenna in a location that provides a free line-of-sight to the tower.
- If you cannot identify the nearest GSM tower of your provider, place the antenna on a higher position; generally, higher is better.
- Use good quality (low-loss) antenna cables. Generally, the thicker the cable, the better.
- Avoid unnecessary adaptors and connectors in the antenna cable, as every "joint" cause a significant signal loss (0.5 to 1 dB).
- Use an antenna with a higher antenna gain. (simple stubby antennas can have a gain of -9db, a rod antenna can have an antenna gain of 0 or 4 dB or higher; Note that the allowed radio power is limited to 1W/2W. An antenna with a higher gain is only allowed when this only compensates for the cable and connector losses).
- Seal your antenna-connector with vulcanizing tape, to prevent from oxidation.
- When the integrated antenna is used, make sure that the data logger is NOT mounted on a metal plate.
- **When the data logger is encapsulated in a metal enclosure or cage of faraday, you may NOT use the integrated antenna, but you must use an external antenna to avoid damaging the MODEM.**

Make sure the SIM you intend to use is compatible with your network and the pin code protection is disabled.

6 Maintenance and Repair

6.1 RTC Lithium Battery replacement

The battery of the data logger is designed to last for the lifetime of the instrument. It should not be necessary to replace this battery.

6.2 Recalibration

Calibration of the data logger has been performed while manufacturing. YDOC guarantees the calibration to last for 2 years. However in most cases the calibration will last for the lifetime of the instrument. Calibration is important for high accuracy measurements and in situations where time stamping is very important. The logger has a NTP-time-synchronize option, which is selectable by the user. The parts of the data logger that could need re-calibration are:

- Analog inputs
- Real time clock

For most applications, the analog inputs are sufficiently accurate, and need no re-calibration for the lifetime of the instrument. But in special cases, where the user demands a high precision measurement, the analog interface may be re-calibrated after that period. High temperature deviations and harsh environment are factors that needed to be considered. Please contact your local supplier for more information on recalibration needs and –support. The real time clock is also calibrated during the manufacturing process, and has very good long life stability (see spec. sheet). Also, when operating in a harsh environment, the need for a recalibration can be applicable. YDOC can perform overall calibrations any time you like.

6.3 XRAY

In the uncommon event of exposure to XRAY, extra precautions are needed. When the device is shipped many times, and is scanned for a security check, the analog input calibration will be harmed. Although the level of radiation is very low, the data logger can be harmed if the number of times that it is exposed to radiation exceeds 10. What will happen is that the analog interface will drift outside its spec's. As a precaution the user can shield his device, with a metal can, to prevent from damage. Normally, the impacts of these security-scans are very low and cause no problems.

7 Safety

Don't work on the wiring of the data logger when powered from an external supply.

7.1 Power supply

The data logger is protected against reversed polarity of the battery power. The mains power supply is protected by a 4AT fuse type TR5.

7.2 ESD

The data logger is equipped with an ESD (Electronic Static Discharge) protection on all "outside world" leads. i.e. comports and analog inputs etc. Though it is designed to withstand a certain amount of electrical discharge (human body model) it is strongly advised to take precautions while operating or servicing the data logger.

8 Environment and disposal

The data logger is manufactured in compliance with the RoHS directive (Reduction of Hazardous Substances) EU directive 2002/95/EC, which means in popular terms that the product is "lead-free".

When the data logger is taken out of service, dispose the data logger in accordance to the local regulations at the time the product is disposed.

Regulations for disposal of batteries may be different. Remove the batteries and dispose them in accordance to the local regulations for batteries.

9 Transport and Storage

The following requirements are applicable for transport and storage of the data logger.

Storage:

Humidity	< 95% (Non condensing)
Temp	10 .. 30 °C

Transport:

Humidity	< 95% (Non condensing)
Temp	10 .. 30 °C

If the data logger is delivered in its standard protecting enclosure, it is strongly recommended to use this case for all transportation, until the final location of operation. This enclosure is especially designed to protect the data logger from being damaged.

10 Appendix

10.1 Specifications

Power Supply			
Protection	Power reverse polarity protection		
Input Range	0.8 ~ 5 Vdc		
Type of Power	Battery		
Power Consumption *	Sleep mode	Operating mode	Send mode
	360 uW 100 uA @ 3.6 Volts	180 mW 60 mA @3.6 Volts	~1 Watt ~ 300 mA @ 3.6 Volts
General Environment			
Temperature	Operating: -30 ~ + 75 °C; Storage -40 ~ +85 °C		
Humidity	5 ~ 100 % RH		
IP Protection	IP 67 (When used in the original case)		
Operation			
Battery life	up to 10 years; consult user manual for more information		
Configuration Programming	Via USB port ; no special software needed; uses hyperterminal or other terminal program		
Data Retrieval	Manually exchange micro SD-card; Automatic via GPRS (Email / FTP / Native protocol) Via USB-Connection by means of a Computer (Windows)		
Alarming	On pre-defined thresholds of measurements; Via SMS, Email		
PowerSwitch	Internal voltage convertor for supplying remote sensors ; 100 mA @ 12 Volts		
System			
CPU	ARM Cortex M3		
Clock Frequency	72 Mhz		
Watchdog	Yes		
RTC(Real Time Clock)	Yes, internally calibrated; accuracy < 100 ppm; Battery Backuped		
FLASH Memory	512 KB		
SRAM	64 KB		
NVRAM	84 bytes , battery backup, data valid up to 20 years		
Analog inputs	12 bits		
Temperature sensor	Yes		
Power Sensor	Yes, Monitors power consumption, rest-capacity of battery		
Expansion Bus	One, for optional modules. Extra I/O, GPS, future functionality		
USB port	USB 2.0 full speed interface		
Sample Frequency	max 4 Hz		
Datalog Frequency	max 4 Hz		
Rohs Compliant	Yes		
Analog Inputs			
Number of Single Ended Channels	4		
Resolution	12 bits		
Input type	0 ~ 20 mA (Channel 1 to 4) 0 .. 10 V (MLx15-xxx only)		
Number of Differential Channels	2 (ML-2013 only)		
Resolution	16 bits		
Input type	Voltage 0 - 2000 mV , 8 different ranges. Smallest detectable step <1 uV		
Memory Card			
Type	micro-SD		
Capacity	4 GB (other sizes possible)		
Filesystem	FAT 32		
Communication Ports			
SER1	RS232; TxD, RxD; Non-isolated;Enhanced ESD Specification: ±15kV Human Body Model; Speed: 115200 bps max. (230kbps on request)		
	RS485		
	SDI12		
SER2	RS232; TxD, RxD; Non-isolated;Enhanced ESD Specification: ±15kV Human Body Model; Speed: 115200 bps max. (230kbps on request)		
Counter input			
Type	Four Digital input 0 ~ 3.6 Volts; Internal pull up & down; 50 kHz max. storage of value in Non Volatile Ram, even after battery replacement.One input is coil input (high sensitive mV range)		
GPRS / GSM Modem			
Frequency Range	Quad Band EGSM 850 / 900 / 1800 / 1900 MHz		
Capabilities	GPRS / GSM / FTP / EMAIL / SMS		
GPS			
GPS Option Module	Option: not included . See manual		
Dimensions PCB			
W x H	148 x 72 mm (ML-2012), 110 x 90 mm (ML-2013)		
Weight PCB			
Netto Weight	70 Grams (ML-2012), 52 grams (ML-2013)		

* The Power consumption in sleep mode is when Datalogger is idle, and no tasks performing. Only the RTC is running

10.2 CE Declarations of Conformity



EU Declaration of Conformity

Swammerdamlaan 14
6721 BK Bennekom
www.ydoc.biz
info@your-data-our-care.com

(in accordance with ISO/IEC 17050)

Your Data Our Care

We,

Your Data Our Care

This Declaration of Conformity is in accordance with the European Standard EN ISO/IEC 17050:2010 Conformity Assessment

"Supplier's confirmation of conformity"

The basis for the criteria has been found in international documentation, particularly in ISO/IEC.

This declaration is an EC Type Declaration of Conformity as referenced in EC directive 2014/30/EU The EMC-directive and as in Appendix III.B

declare under our sole responsibility that the product:

Type ML-2013 Low Power GPRS Datalogger

The object of the declaration described above is in conformity with the relevant EU harmonization legislation: at date of this declaration:

2014/30/EU The Electromagnetic Compatibility Directive (EMCD)

2011/65/EU The Restriction of Hazardous Substances Directive (RoHS)

Standards used during compliance assessment:

EN 61326-1:2013 Electrical equipment for measurement, control and laboratory use- EMC requirements - for use in industrial locations

EN 61000-6-1:2001

EN61000-6-3:2001

The product uses a Teitl GPRS/UMTS/2G/3G Module type UL-865-XXX (for ML315 datalogger) and GL-865QUAD-V3 for ML215 datalogger, which is tested by the manufacturer and also notified bodies, registered under (nobo) number: 1909

Almere, 3-4-2017

R. Kleine	
Technical Director	
Signature:	



EU Declaration of Conformity

Swammerdamlaan 14
6721 BK Bennekom
www.ydoc.biz
info@your-data-our-care.com

(in accordance with ISO/IEC 17050)

Your Data Our Care

We,

Your Data Our Care

This Declaration of Conformity is in accordance with the European Standard EN ISO/IEC 17060:2010 Conformity Assessment

"Supplier's confirmation of conformity"

The basis for the criteria has been found in international documentation, particularly in ISO/IEC.

This declaration is an EC Type Declaration of Conformity as referenced in EC directive 2014/30/EU The EMC-directive and as in Appendix III.B

declare under our sole responsibility that the product:

Type ML-x15xxx Low Power GPRS Datalogger

Models:

ML-215DS-LI, ML-215AD-LI, ML-215ADS-LI,
ML-215DS-PV, ML-215AD-PV, ML-215ADS-PV,
ML-315DS-LI, ML-315AD-LI, ML-315ADS-LI,
ML-315DS-PV, ML-315AD-PV, ML-315ADS-PV
ML-215DS-DC, ML-215AD-DC, ML-215ADS-DC, ML-215TFT,
ML-315DS-DC, ML-315AD-DC, ML-315ADS-DC, ML-315TFT

The object of the declaration described above is in conformity with the relevant EU harmonization legislation: at date of this declaration:

2014/30/EU The Electromagnetic Compatibility Directive (EMCD)

2011/65/EU The Restriction of Hazardous Substances Directive (RoHS)

Standards used during compliance assessment:

EN 61326-1:2013 Electrical equipment for measurement, control and laboratory use-
EMC requirements - for use in industrial locations

EN 61000-6-1:2001

EN61000-6-3:2001

The product uses a Teitit GPRS/UMTS/2G/3G Module type UL-865-XXX (for ML315 datalogger) and GL-865QUAD-V3 for ML215 datalogger, which is tested by the manufacturer and also notified bodies, registered under (nobo) number: 1909

Almere, 3-4-2017

R. Kleine	
Technical Director	
Signature:	



EU Declaration of Conformity

Swammerdamlaan 14
6721 BK Bennekom
www.ydoc.biz
info@your-data-our-care.com

(in accordance with ISO/IEC 17050)

Your Data Our Care

We,

Your Data Our Care

This Declaration of Conformity is in accordance with the European Standard EN ISO/IEC 17060:2010 Conformity Assessment

"Supplier's confirmation of conformity"

The basis for the criteria has been found in international documentation, particularly in ISO/IEC.

This declaration is an EC Type Declaration of Conformity as referenced in EC directive 2014/30/EU The EMC-directive and as in Appendix III.B

declare under our sole responsibility that the product:

Type WDL-x14xx-LI Low Power GPRS Datalogger

Models:

WDL-214AD-LI, WDL-214DS-LI, WDL-314AD-LI, WDL-314DS-LI, WDL-N314AD-LI, WDL-N314DS-LI

The object of the declaration described above is in conformity with the relevant EU harmonization legislation: at date of this declaration:

2014/30/EU The Electromagnetic Compatibility Directive (EMCD)

2011/65/EU The Restriction of Hazardous Substances Directive (RoHS)

Standards used during compliance assessment:

EN 61326-1:2013 Electrical equipment for measurement, control and laboratory use- EMC requirements - for use in industrial locations

EN 61000-6-1:2001

EN61000-6-3:2001

The product uses a Teitl GPRS/UMTS/2G/3G Module type UL-865-XXX (for ML315 datalogger) and GL-865QUAD-V3 for ML215 datalogger, which is tested by the manufacturer and also notified bodies, registered under (nobo) number: 1909

Almere, 3-4-2017

<i>R. Kleine</i>	
<i>Technical Director</i>	
<i>Signature:</i>	



EU Declaration of Conformity

Swammerdamlaan 14
0721 BK Bennekom
www.ydoc.biz
info@your-data-our-care.com

(in accordance with ISO/IEC 17050)

Your Data Our Care

We,

Your Data Our Care B.V.

This Declaration of Conformity is in accordance with the European Standard EN ISO/IEC 17050:2010 Conformity Assessment "Supplier's conformation of conformity"

The basis for the criteria has been found in international documentation, particularly in ISO/IEC.

This declaration is an EC Type Declaration of Conformity as referenced in EC directive 2014/30/EU The EMC-directive and as in Appendix III.B

declare under our sole responsibility that the product:

Type ML-x17xxx Low Power GPRS Datalogger

Models:

ML-217DS-LI, ML-217AD-LI, ML-217ADS-LI,
ML-217DS-PV, ML-217AD-PV, ML-217ADS-PV,
ML-317DS-LI, ML-317AD-LI, ML-317ADS-LI,
ML-317DS-PV, ML-317AD-PV, ML-317ADS-PV
ML-417DS-LI, ML-417AD-LI, ML-417ADS-LI,
ML-417DS-PV, ML-417AD-PV, ML-417ADS-PV
ML-217DS-DC, ML-217AD-DC, ML-217ADS-DC, ML-217TFT,
ML-317DS-DC, ML-317AD-DC, ML-317ADS-DC, ML-317TFT,
ML-417DS-DC, ML-417AD-DC, ML-417ADS-DC, ML-417TFT,

The object of the declaration described above is in conformity with the relevant EU harmonization legislation: at date of this declaration:

2014/30/EU The Electromagnetic Compatibility Directive (EMCD)

2014/53/EU The Radio Equipment Directive (RED) (formerly R&TTE 99/5/EC)

2014/35/EU The Low Voltage Directive (LVD)

2011/65/EU The Restriction of Hazardous Substances Directive (RoHS)

Standards used during compliance assessment:

EN 61326-1:2013 Electrical equipment for measurement, control and laboratory use-
EMC requirements - for use in industrial locations

EN 61000-6-1:2001

EN61000-6-3:2001


The product uses a Teit GPRS/UMTS/2G/3G/4G Module type xE-910-XXX, which is tested by the manufacturer and also notified bodies, registered under (nobo) number: 1909

Zeewolde, 0-11-2017

R. Kleine	
Technical Director	
Signature:	

10.3 Open Collector output

In electronics a common way of driving external loads is the use of an “open collector” output. This is a transistor, with its collector left unconnected, for the benefit of user to connect to its load of interest. The open collector (o.c.) is very versatile, and provides the possibility to use various voltages.

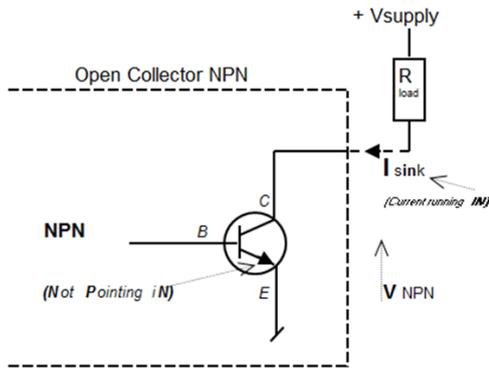

If the NPN transistor is **OFF**, I_{sink} equals 0 mA.
This means that V_{NPN} equals approx. + V_{Supply} .

If the NPN transistor is **ON**, I_{sink} equals approx. $(+V_{supply} / R_{load})$.
This means that V_{NPN} equals 0 V.

24 volt source, pull down to 0 volts



In the picture above, an open collector output is shown. The o.c. is only capable of sinking current and NOT sourcing current. That’s why the “load” in the picture above is located in the “high side”. The transistor will sink the bottom side of the “load”, enabling current to flow through.


The user can choose his own voltage level, because the transistor only acts as a switch and NOT supplying any voltage. In your YDOC data logger the maximum “supply voltage” for the o.c. switch is limited to 40 volts DC.

10.3.1.1 Using a relay to drive an external load

If you like a relay, in order to switch an external “load”, please bear in mind that a relay can produce very high these spikes to occur, always use a diode, connected in parallel with the “load” .

Picture below shows how to do this.

The transistor and resistor shown, are part of the data logger PCB.

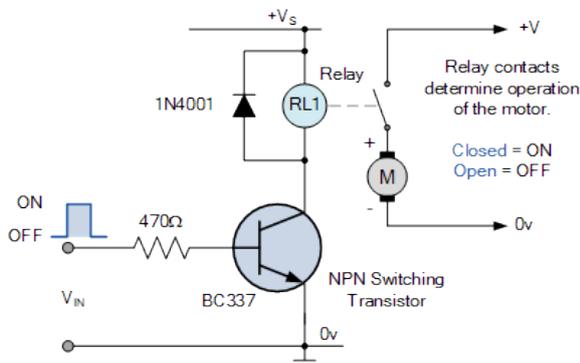

10.4 Trouble shooting

If you encounter problems with the data logger, you can start checking the following.

- First try to set up a connection, via USB, and use the program, YDOC-terminal, to communicate with it.
- If that doesn't work, you have to check the battery-power, so you have to open the case. Do this in a dry and clean environment, NOT in the field. Normally a flat battery is preceded by an alarm-message.
- Check the fuse

Most parts of the data logger are tested at startup. To monitor the messages which are issued at startup, you have to connect a PC/terminal to the debug port.



Attention:

The default DEBUG port is serial port 1, but when a sensor is connected to this port, the DEBUG port becomes port 2. If both ports are in use, you can use the USB port as debug port, but you won't be able to see startup-messages. In this case it is advised to remove a sensor from the configuration, temporarily.



```

YDOC Logger Version 1.6 Build 1
<12:20:05>
2012/10/07 12:20:05
Init User Interface
Init Modem Interface
Init SD-card
File system OK
Init System Monitor
Start up from Power on
POWER_ON: System log...done
SYS_START: System log...done
Init NTP Time update task
Init Sensors Internal
Init Sensor GSM signal
Init Email
Init TCP
Running
    
```

These are typical start up messages:

Explanation:

The data logger starts and initializes its peripherals. First, an overview of the firmware version is given with a timestamp. This timestamp should be accurate, carefully check the timestamp. If it is slightly wrong, it must be adjusted. If it is totally out of date, it designates a RTC-problem. There should be NO errors on this startup. If there are errors contact your local YDOC-dealer. A screen dump of the startup messages will help to solve the problem.

```

YDOC Logger Version 1.6 Build 1
<12:29:21>
2012/10/07 12:29:21
Init User Interface
Init Modem Interface
Init SD-card
File system error
Init System Monitor
Start up from Power on
POWER_ON: System log...File system
error
SYS_START: System log...File system
error
Init NTP Time update task
Init Sensors Internal
Init Sensor GSM signal
Init Email
Init TCP
Running
    
```

An example of a defective data logger is given below. This data logger has its micro SD-card not installed. You can clearly notify the problem, by looking at the startup messages.

When there is no debug output visible at all, contact your local YDOC-supplier.

Attention:



Always connect the USB-cable to the PC, even when you are connected to the serial port for debug output. When the data logger is NOT connected by USB, it will switch into low power mode (Auto Sleep), and you won't get any debug data.

10.5 System messages

Meaning of the System messages (S-records in TXT and CSV or \$Msg-lines in JSON data log files)

A System message contains a message code, an optional supplemental code/text and an optional explanatory text.

Please find below a list with possible System messages.

Message code	Supplemental code/text	Meaning	Possible cause/reason
SYS_START	"System name & S/N"	System is started and deployed	At power on, or reset
SYS_DEPLOYED	"System name & S/N"	System is deployed	After a delayed deployment
SYS_UPGRADED	"System name & S/N"	Firmware upgrade detected	After firmware upgrade
CFG_CHANGED	"System name & S/N"	Configuration has changed	After configuration editing
CFG_ERR		Configuration error	Firmware downgrading, or configuration upload with different version
NO_CFG		No configuration detected	Data logger is not yet configured
CFG_UPL	"cause of failure"	Configuration upload failed	Disruption in the data transfer, or SD card failure
FW_UPG	"cause of failure"	Firmware upgrade failed	Disruption in the data transfer, or SD card failure
PVD_DIP	"number"	Power voltage detection dips	When the internal power (temporarily) drops unexpectedly below 2.8V (power has returned before switch off occurred)
SD_FAIL	"number"	Number of temporarily SD card failures	SD card failure
NETWORK	"fallback;2G"	Network fallback (only for 2G+3G Modems)	When 3G network is not available
WDT	"Sensor name"	Shows the sensor driver name were the watchdog timeout occurred	Sensor defect, or wrongly connected, or warmup time too short
WDT	MODEM_INIT	Watchdog timeout while initializing Modem	No response from Modem, or no SIM, or SIM not detected, or PIN on SIM
WDT	NETWORK_REG	Watchdog timeout while trying to register on a network	No response, or (temporarily) no network coverage, or SIM subscription failure (inactive/invalid/blocked or black listed)
WDT	APN_OPEN	Watchdog timeout while trying to find an internet access point	No response, or APN access point name wrong
WDT	APN_LOGIN	Watchdog timeout while trying to login to the internet access point	No response, or APN user or password wrong, or authentication failure
WDT	SERVER_LOGIN	Watchdog timeout while trying to login to the Email/FTP/TCP/HTTP server	No response, or server not available, or credentials wrong
WDT	FILE_OPEN	Watchdog timeout while trying to open a file on the FTP server	No response, or file handling error on the server
WDT	DATA_SENDING	Watchdog timeout while sending data to the Email/FTP/TCP/HTTP server	No response, or unexpected network disruption, or server error
WDT	TCP_RESPONCE	Watchdog timeout while waiting for acknowledge from the TCP/HTTP server	No response, or unexpected network disruption, or server error
WDT	DATA_END	Watchdog timeout while trying to disconnect from the Email/FTP/TCP/HTTP server connection	No response, or unexpected network disruption, or server error
WDT	"STATE number"	Modem state machine step where the watchdog timeout occurred	No response
ERR	"Driver name"	Shows the driver name were an error occurred, with if applicable some additional information	Sensor defect, or unknown failure
ERR	MODEM_INIT	Error while initializing Modem	No SIM, or SIM not detected, or PIN on SIM
ERR	NETWORK_REG	Error while trying to register on a network	(Temporarily) no network coverage, or SIM subscription failure (inactive/invalid/blocked or black listed)

ERR	APN_OPEN	Error while trying to find an internet access point	APN access point name wrong
ERR	APN_LOGIN	Error while trying to login to the internet access point	APN user or password wrong, or authentication failure
ERR	SERVER_LOGIN	Error while trying to login to the Email/FTP/TCP/HTTP server	Server not available or credentials wrong
ERR	FILE_OPEN	Error while trying to open a file on the FTP server	File handling error on the server
ERR	DATA_SENDING	Error while sending data to the Email/FTP/TCP/HTTP server	Unexpected network disruption, or server error
ERR	TCP_RESPONCE	Error while waiting for acknowledge from the TCP/HTTP server	Unexpected network disruption, or server error
ERR	DATA_END	Error trying to disconnect from the Email/FTP/TCP/HTTP server	Unexpected network disruption, or server error
ERR	"STATE number"	Modem state machine step were the error occurred	Unknown
SMS_SEND_ERR		An error occurred while sending SMS	See the Modem ERR/WDT message before for more details
SMS_SEND_OK		Sending of the SMS was successful	
SMS_RECV_ACVA	"Phone number"	An ACVA SMS was received	
SMS_RECV_ERR	"Phone number"	An invalid SMS was received	
CNT_RESET	"digital sensor name"	Shows the reset of the pulse counter	When reset at midnight option is on, or after manual change
STR	"Driver name;raw data"	Shows the raw data log	When this option is enabled (generic serial string and GPS)
TIME_FIX	" +/- number of sec"	Shows the number seconds the internal clock was adjusted	After a NTP time synchronization
TIME_FIX	"Summer time started"	Shows that the clock is adjusted to the start of summer time	When summer time (daylight saving) option is enabled
TIME_FIX	"Summer time ended"	Shows that the clock is adjusted to the end of summer time	When summer time (daylight saving) option is enabled
ALARM_SET	"Code;limit;value"	Shows the parameter code, alarm limit and actual value	When the alarm is raised
ALARM_RESET	"Code;limit;value"	Shows the parameter code, alarm limit and actual value	When the alarm is cleared